


Safety Suite Device Configurator USER GUIDE

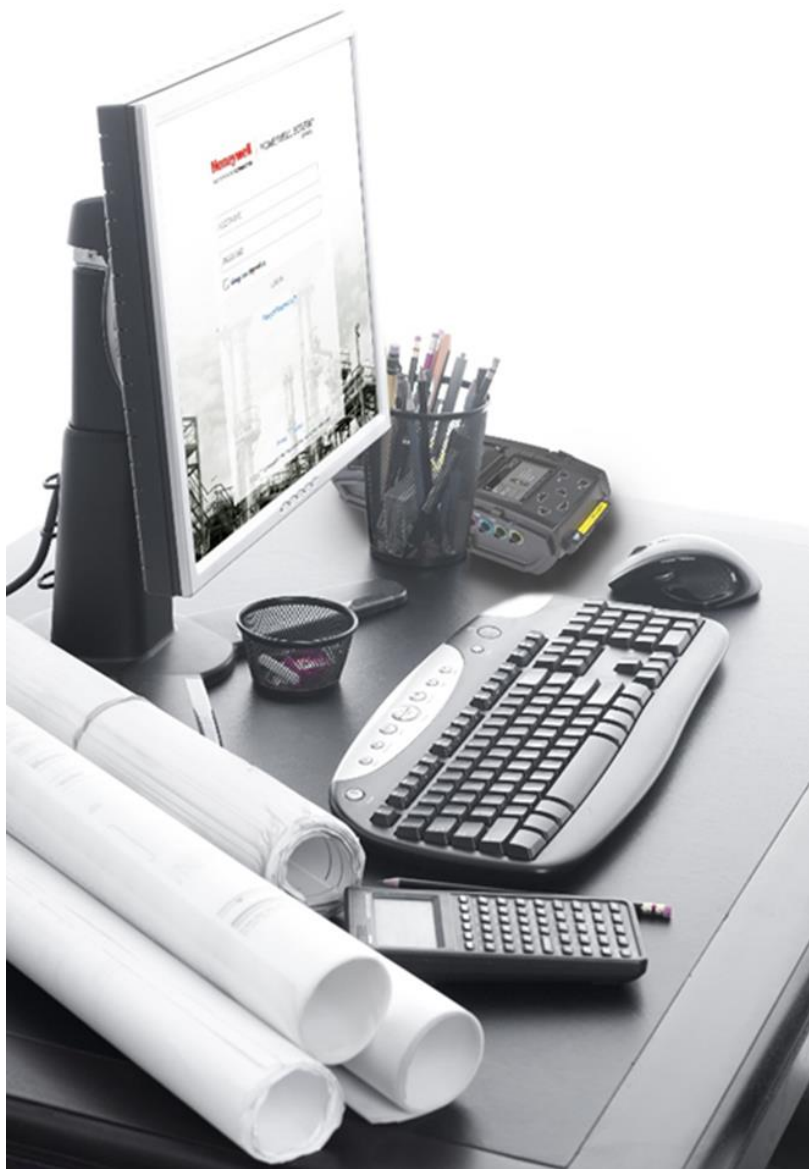

Contents

1	Introduction.....	6
2	Requirements	6
2.1	Hardware	6
2.2	Software.....	6
3	Supported Instruments	7
3.1	IntelliDoX & MicroDock II.....	7
3.2	IntelliDoX.....	7
3.3	MicroDock II	7
3.3.1	BW IR Dongle	7
3.3.2	AutoRAE 2 & Travel Charger.....	7
3.3.3	Direct USB	7
3.4	Migration from Existing software.....	8
3.4.1	Fleet Manager	8
3.4.2	ProRAE Studio II.....	8
3.4.3	IQ Management Software Suite	8
4	Installation	9
5	First Time Start-Up.....	12
5.1	Username	13
5.2	Password.....	14
5.3	Security Questions.....	14
5.4	Software Registration	15
6	Connecting an Instrument to Your Computer	16
6.1	Connection via IntelliDoX	16
6.2	Connection via AutoRAE 2.....	17
6.3	Connection via MicroDock II.....	17
6.4	Microdock-view /save config from file	17
7	Security.....	22
7.1	Data Security	22
7.2	Wireless Security Warning	22
8	Starting Safety Suite Device Configurator from the Desktop	23
9	Logging In.....	23
9.1	Password Recovery for Non-Administrators	24
9.2	Password Recovery for Administrators	25
9.3	Password expiry	26
9.4	Login Process.....	28

10	Title Bar/Quick-Access Toolbar	29
10.1	Registrations	29
10.2	Devices	29
10.3	Download Status.....	30
10.4	Role Information	30
10.4.1	Role Name.....	31
10.4.1.1	Role Names and Access Levels.....	31
10.4.2	Edit Profile	31
10.4.2.1	Update Profile Picture.....	32
10.4.2.2	Personal Information.....	33
10.4.2.3	Change Password.....	33
10.4.2.4	Update Security Questions.....	33
10.4.3	Sign Out.....	33
10.4.4	Settings.....	34
10.4.4.1	Product Services.....	35
10.4.4.2	Service Ports.....	36
10.4.4.3	Local Settings	36
10.4.5	User Role List.....	36
10.5	Help.....	37
11	Views.....	37
11.1	Devices	38
11.1.1	Device Hierarchy	39
11.1.2	Sorting and Organization	39
11.1.2.1	Sort by.....	39
11.1.2.2	Columns.....	40
11.1.2.3	Refresh.....	40
11.1.2.4	List View.....	41
12	Assign Device to Worker.....	41
13	Filter by.....	42
13.1	Connection	43
13.2	Devices	45
13.3	Assigned To.....	45
13.4	Last Communication	45
13.5	First Communication.....	46
13.6	Actions	47
13.6.1	View the list of Devices.....	47
13.6.2	Device Details	48

13.6.2.1	Instruments	49
13.6.2.2	Docking Stations	50
13.6.2.2.1	Menu Passcode	51
13.6.2.2.2	Edit Gas Cylinder Configuration	51
13.6.2.3	Device History	52
13.6.2.3.1	Filters	53
13.6.2.4	Sensors	56
13.6.2.5	Settings	57
13.6.3	Custom fields in Device Configurator	58
13.6.4	Download Data	62
13.6.4.1	Data download from Multiple Intellidox	62
13.6.4.2	Scheduled data import	63
13.6.5	Archive Device	67
13.6.6	Network Passcode	67
13.7	Save Template	68
13.7.1	Templates	68
13.8	IntelliDoX USB Data Download	70
13.9	IntelliDoX USB Configuration Management	71
13.10	User List	72
13.10.1	Sort by	73
13.10.2	Columns	73
13.10.3	Actions	74
13.10.4	Add A User	75
13.10.5	Filter By	76
13.10.5.1	Status	76
13.10.5.2	Name	77
13.10.5.3	Device Assigned	78
13.10.5.4	User Role	79
13.10.5.5	Username	79
13.10.6	Add A User	80
13.10.7	Profile Picture	81
13.11	Generate Report	82
13.11.1	Report header	84
13.11.2	Multidevice reports-Eventlog(Multidevice event report)	87
14	Uninstall Safety Suite Device Configurator	90
14.1	Delete Instrument Data (Optional)	91

14.1.1	Uninstall Microsoft SQL Server 2012.....	91
15	Migrating ProRA E Studio Database to Safety Suite Device Configurator	96
16	Migrating Fleet Manager Database to Safety Suite Device Configurator	98
17	Migrating IQ Manager Database to Safety Suite Device Configurator	100
17.1	Backup of Source Files.....	102
18	Migrating IQ Manager Database to Safety Suite Device Manager	103
19	Device Configurator FAQs.....	104
19.1	General Questions.....	104
19.2	Installation.....	106
19.3	Login.....	110
19.4	Device Inventory.....	112
19.5	Device Data Download.....	114
19.6	Device Configuration.....	115
19.7	Device History.....	115
19.8	User Management.....	116
19.9	Data Migration.....	117
19.10	Firmware.....	120
19.11	Passcode.....	122
19.12	Language Support.....	123
19.13	Device Registration.....	123
19.14	Event Report.....	124

1 Introduction

Safety suite Device Configurator software allows data logs and configuration settings from supported Honeywell instruments to be downloaded to a computer, and configurations to be uploaded from a computer to the instruments. Templates can be created, saved, and edited, as well as user/instrument references.

Safety suite Device Configurator communicates with supported instruments via supporting docking stations and USD direct connection when configuring them or retrieving their data logs or event logs. Refer to your product's manual for details on connecting with a computer, as well as all safety requirements.

This version of the software allows you to:

- Download data logs
- Download configuration settings
- Change and upload new configurations settings
- Update firmware
- Download reports
- Create, edit, store, and upload templates
- Upload historical data from Fleet Manager

2 Requirements

2.1 Hardware

CPU	:1GHz or better
Monitor	:Color Monitor with resolution of at least 1024 x 768,16-bit color
Memory (RAM)	:2GB
Disk Space	:At least 4GB of free space

2.2 Software

Operating System: Windows 7 (32-bit and 64-bit), and Windows 10 (64-bit).

3 Supported Instruments

3.1 IntelliDoX & MicroDock II

- BW Clip & BW Clip Real Time
- BW MicroClip XL & BW MicroClip X3

3.2 IntelliDoX

- BW Clip4
- BW Solo
- BW Ultra

3.3 MicroDock II

- BW MaxXT II
- BW Quattro
- GasAlertMicro 5

3.3.1 BW IR Dongle

- BW MaxXT II
- BW MicroClip XL & BW MicroClip X3
- BW Quattro
- BW Ultra

3.3.2 AutoRAE 2 & Travel Charger

- MicroRAE
- MiniRAE 3000 & MiniRAE Lite
- MultiRAE, MultiRAE Lite & MultiRAE Pro
- ppbRAE 3000
- QRAE 3
- ToxiRAE Pro, ToxiRAE Pro CO₂, ToxiRAE Pro LEL & ToxiRAE Pro PID
- UltraRAE 3000

3.3.3 Direct USB

- AreaRAE Plus & AreaRAE Pro

3.4 Migration from Existing software

3.4.1 Fleet Manager

- BW Clip & BW Clip Real Time
- BW Clip4
- BW MaxXT II
- BW MicroClip XL & BW MicroClip X3
- BW Quattro
- BW Ultra
- GasAlert Extreme
- GasAlertMicro 5

3.4.2 ProRAE Studio II

- AreaRAE Plus & AreaRAE Pro
- MicroRAE
- MiniRAE 3000 & MiniRAE Lite
- MultiRAE, MultiRAE Lite & MultiRAE Pro
- ppbRAE 3000
- QRAE 3
- ToxiRAE Pro, ToxiRAE Pro CO₂, ToxiRAE Pro LEL & ToxiRAE Pro PID
- UltraRAE 3000

3.4.3 IQ Management Software Suite

- ToxiPro


4 Installation

Download Safety Suite Device Configurator from


<https://pages8.honeywell.com/safetysuite-device-configurator.html#download>

1. Double-click on the filename, and start the installation process. During installation of Device Configurator, the user can select the appropriate locale based on their region and system settings. As shown in the below screen, while installing the Device Configurator user must select the **locale** where installation should happen, select the languages in the drop-down bar and click next to continue to install device configurator. The default locale is English (United states).

Please note: This setting will apply to dates and number formats only. The application would be displayed in English.

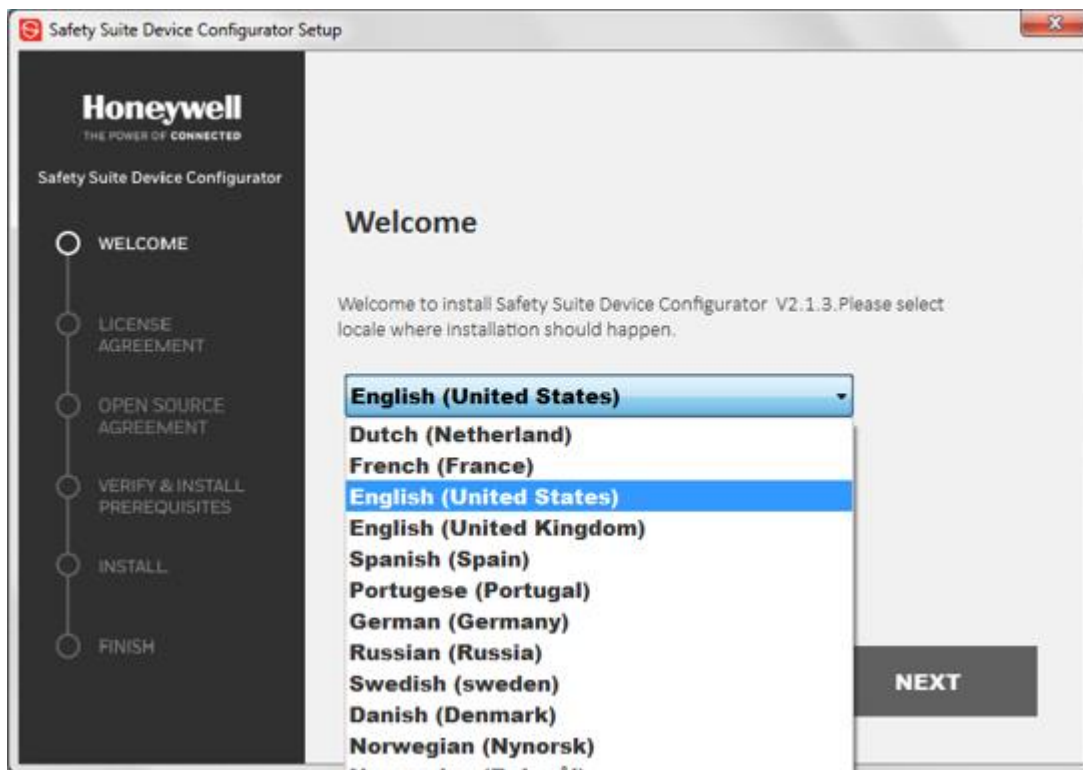


2. Click "Next."

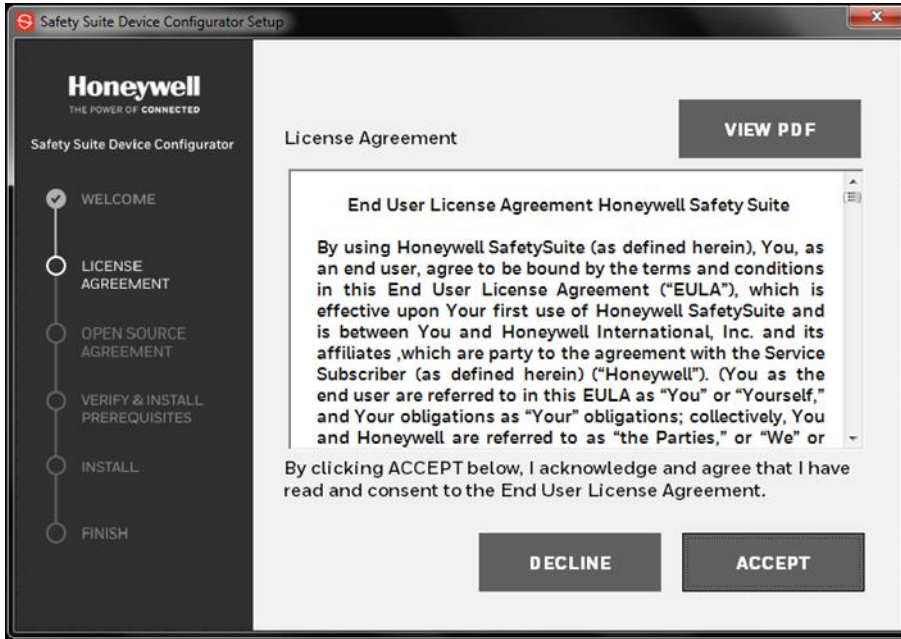

Click “Accept” if you accept the terms (you may also view a PDF of the End User License Agreement).


Next, you see the Open Source License Agreement:

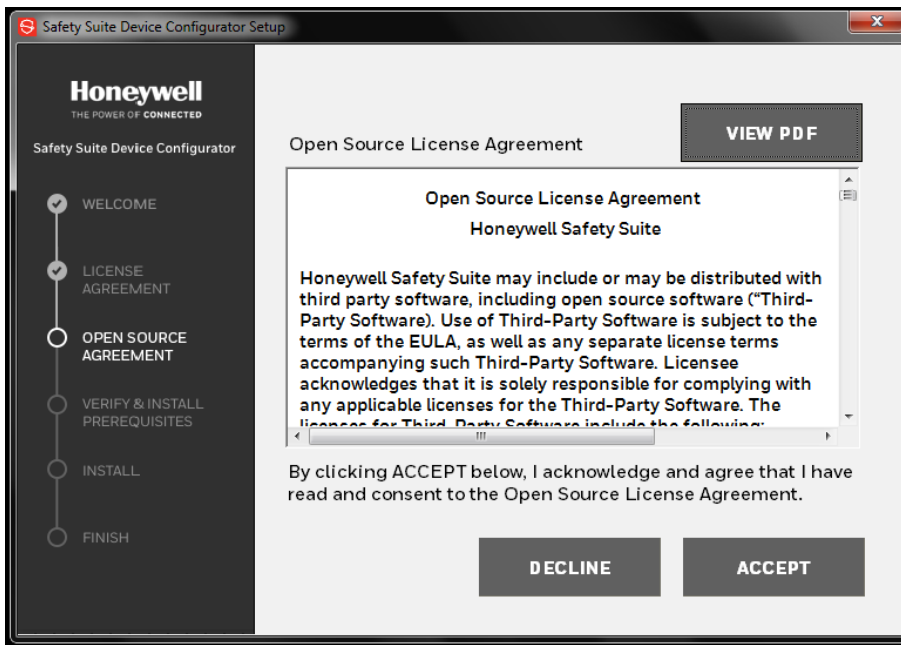


3. Click “Accept” if you accept the terms (you may also view a PDF of the Open Source License Agreement).

If there are any software pre-requisites (.net framework, Microsoft SQL Server), you will be prompted. Install the required prerequisites and continue.


4. Click “Next” to start the installation process. Installation is automatic and takes several minutes.
5. When it stops, click “Next.” Then this screen is shown:

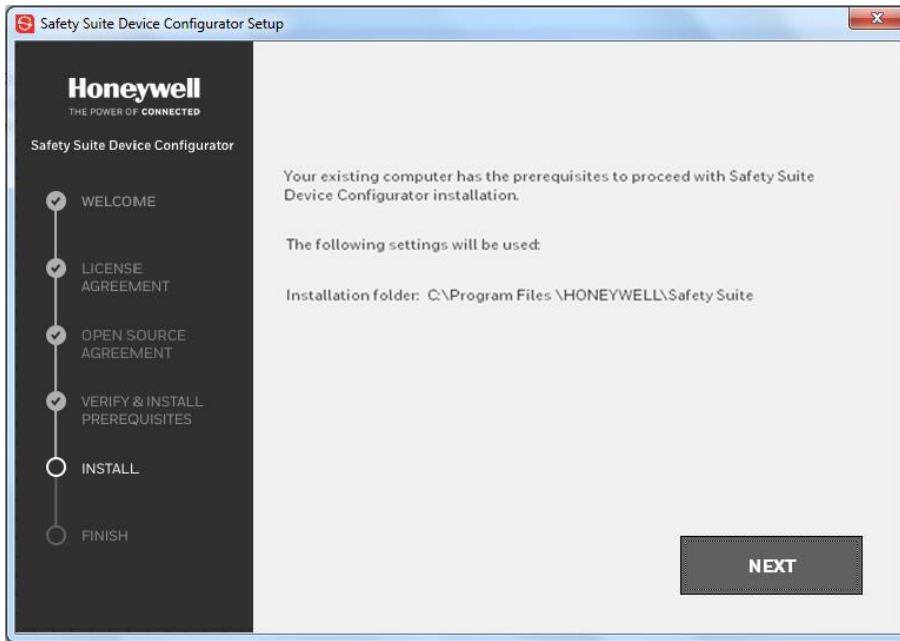

6. Click “Next” to begin the second part of installation.

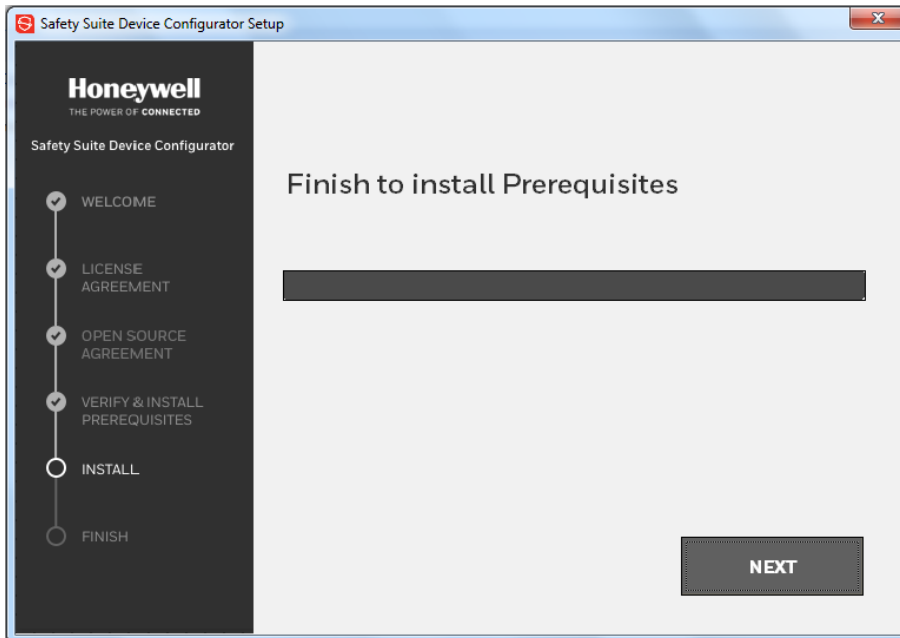

Next, it shows this window to let you know configuration is going on. When the installation is complete, this window appears:

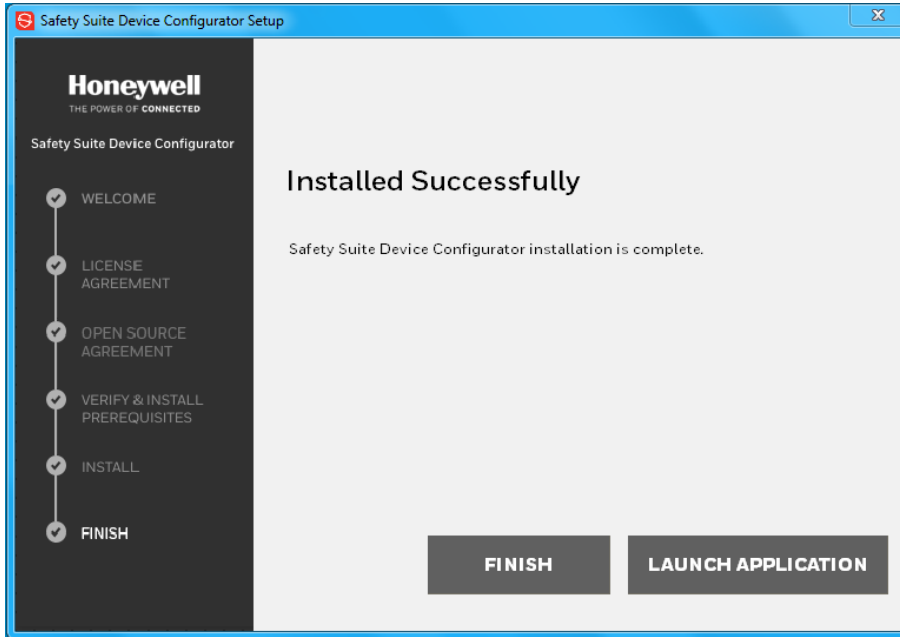

7. Click “Finish” and the installation is complete, and the program exits. Otherwise, click “Launch Application” to finish and then immediately launch Safety Suite Device Configurator.

Note: If you want to uninstall Safety Suite Device Configurator or its SQL server, refer to page 90

5 First Time Start-Up


You should see the Safety Suite Device Configurator icon on your computer’s desktop. Click it to start.




The Legal Agreement is shown, and you must click the box acknowledging that you have read the terms.

You must scroll to the end of the text, using the scrollbar to the right. Then click “I have read and accept the terms and conditions.” Finally, click “Accept” to begin.

Next, you must perform the same process to acknowledge and accept licenses for third-party software. Scroll down, click “I have read and accept the terms and conditions.” and then click “Accept.”

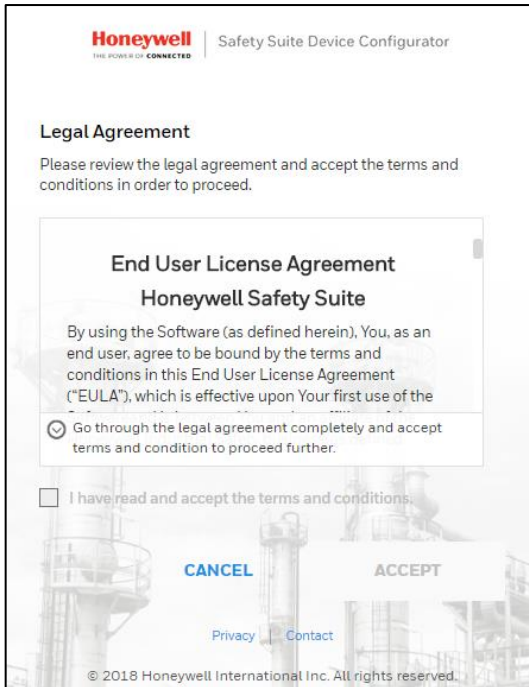

Next is account activation. The first time you log in is different than future logins. You must create a Username and Password. Follow the rules outlined to the right of these fields. Then you must fill in answers to the security questions.

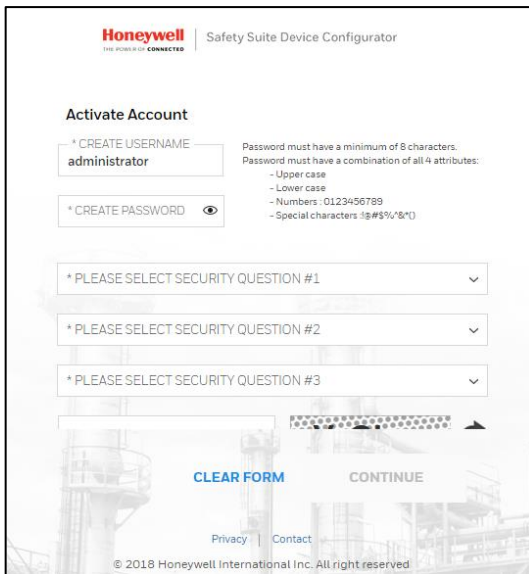

Be sure to scroll down and complete the process.

5.1 Username

You must create a username, which will be used each time you log in to Safety Suite Device Configurator.

5.2 Password

You should change the password every 90 days. You must supply the current password and then type the new password. The password must follow these rules:

- The password must have a minimum of 8 characters.
- The password must include at least one character from all the following types:
 - UPPERCASE
 - lowercase
 - Number: 0 1 2 3 4 5 6 7 8 9
 - Special character, including: ! @ # \$ % ^ * ()

5.3 Security Questions


In case you ever forget your password and want to reset it, you will have to answer security questions. Here is where you put the answers that must be matched if you want to regain access after forgetting your password.

1. Select a security question from each pull-down list.
2. Type in an answer for each of the questions.
3. Click "Update".

In case you should ever forget your password, you will have to answer security questions for access. Here is where you put the answers to the security questions.

1. Select a security question from each pull-down list.
2. Type in an answer for each of the questions.

After you establish a username and password, type the letters showing in the box, following the same format of capital and lower-case letters. You can refresh this by clicking the circle/arrow image to its right.

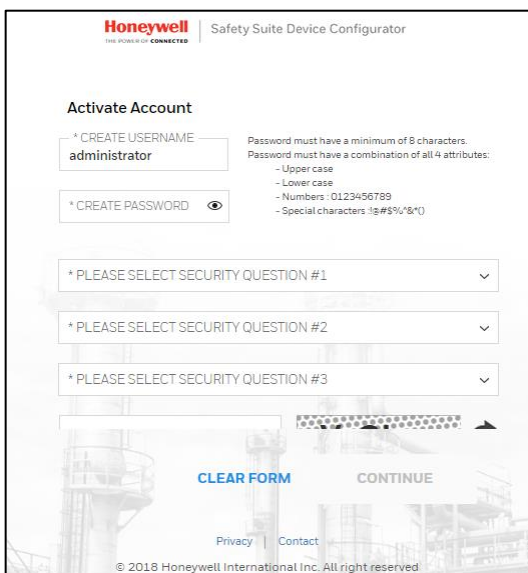

The screenshot shows the 'Activate Account' section of the Honeywell Safety Suite Device Configurator. It includes a username field with 'administrator' entered, a password field with an eye icon, and three dropdown menus for security questions. The password field has a tooltip with requirements: 'Password must have a minimum of 8 characters. Password must have a combination of all 4 attributes: - Upper case, - Lower case, - Numbers: 0123456789, - Special characters: !@#%&^*()'. At the bottom, there are 'CLEAR FORM' and 'CONTINUE' buttons, and a footer with '© 2018 Honeywell International Inc. All right reserved'.

Scroll down and fill in the rest of the information, including typing the case-sensitive text in the Captcha.

The screenshot shows the 'Activate Account' section of the Honeywell Safety Suite Device Configurator. The form includes the following fields and elements:

- Header:** Honeywell logo and 'Safety Suite Device Configurator'.
- Account Name:** A text box containing 'D.A.V Public School'.
- Security Question #2:** A dropdown menu with the question 'What is your favorite food?' and a selected option 'Pasta'.
- Security Question #3:** A dropdown menu with the question 'What was your first pet's name?' and a selected option 'Bruno'.
- Captcha:** A text box containing 'VaGhqc' and a corresponding image of the same text with a refresh icon.
- Buttons:** 'CLEAR FORM' and 'CONTINUE' buttons.
- Footer:** 'Privacy | Contact' and '© 2018 Honeywell International Inc. All right reserved'.

If all information is accepted and you submit the correct letters, then the “Continue” button is highlighted.

Click the “Continue” button.

5.4 Software Registration

Register your software before you begin using Safety Suite Device Configurator.

The screenshot shows the 'Register Your Software' form. It includes the following sections and fields:

- Header:** 'Register Your Software'.
- Message:** 'Congratulations! You have successfully installed Safety Suite™ DeviceConfigurator 1.2.0.845.' and 'Please register to receive future updates, complimentary product information, customer support, latest firmware notifications, one click firmware update etc.'
- Company Name:** A text box with a 100/100 char. remaining indicator.
- First Name:** A text box with a 40/40 char. remaining indicator.
- Last Name:** A text box with a 40/40 char. remaining indicator.
- Company Address:** Two text boxes for 'ADDRESS LINE 1' and 'ADDRESS LINE 2', both with 150/150 char. remaining indicators.
- Button:** A blue 'REGISTER' button.

Fill in the information, and then scroll down to complete the process. Make sure you fill in all information in fields marked with an asterisk (*).

Register Your Software

Congratulations!
You have successfully installed Safety Suite™ DeviceConfigurator 1.2.0.845.

Please register to receive future updates, complimentary product information, customer support, latest firmware notifications, one click firmware update etc.

139/150 char. remaining

* CITY * COUNTRY / REGION

22/30 char. remaining

* POSTAL / ZIP CODE * STATE

25/30 char. remaining

Contact information

* CONTACT EMAIL * PHONE NUMBER


email@domain.com, 50 char. 21/30 digits remaining

WEBSITE

REGISTER

When you have provided sufficient information, the “Register” button is blue. You can now click it to register.

Once registration is complete, this message is shown:



Safety Suite Device Configurator is ready to use.

6 Connecting an Instrument to Your Computer

Your instrument must be connected via wire (USB or Serial) to the computer, turned on, and in communication mode to transmit and receive data via Safety Suite Device Configurator.

Different instruments require different connection methods to connect to a PC. Follow the instructions in the user’s guide that accompanies the instrument, ensuring that you use the correct cable and communication method. In addition, you should make sure the instrument’s battery is charged.

6.1 Connection via IntelliDoX

Follow this procedure for reading data from an IntelliDoX:

1. Connect one end of an Ethernet cable (refer to the IntelliDoX User’s Guide for connection and configuration information) to the IntelliDoX and the other end to a PC running Safety Suite Device Configurator software or the local network in case the dock needs to communicate with the software over the network.
2. Make sure the IntelliDoX has power and is turned on.
3. Start Safety Suite Device Configurator software on the PC.

4. Add IntelliDoX IP to Safety Suite Device Configurator using the settings option. For more information, please refer the “[Product Services](#)” section.
5. Network Passcode is applicable/available on IntelliDoX device having firmware 9.0 and above only. So, before you perform the next step please set a passcode. For more information please refer “[Network Passcode](#)” section.

6.2 Connection via AutoRAE 2

Follow this procedure for reading data from an AutoRAE 2 Controller:

1. Connect a USB cable (or use an Ethernet cable or Wi-Fi; refer to the AutoRAE 2 User’s Guide for connection and configuration information) to the AutoRAE 2 Controller and to a PC running Safety Suite Device Configurator software.
2. Make sure the AutoRAE 2 Controller has power and is turned on.
3. Start Safety Suite Device Configurator software on the PC.
4. Add AutoRAE IP (if connected through network) to Safety Suite Device Configurator using the settings option. For more information, please refer the “[Product Services](#)” section



6.3 Connection via MicroDock II



Follow this procedure for reading data from a MicroDock II:



1. Connect a USB cable to the MicroDock II and to a PC running Safety Suite Device Configurator software.
2. Make sure the MicroDock II has power and is turned on.
3. Start Safety Suite Device Configurator on the PC.

6.4 Microdock-view/save config from file


Users can view and update configuration data for Microdock using a file. The application opens the configuration file and displays the configuration available in the file by Device Type.

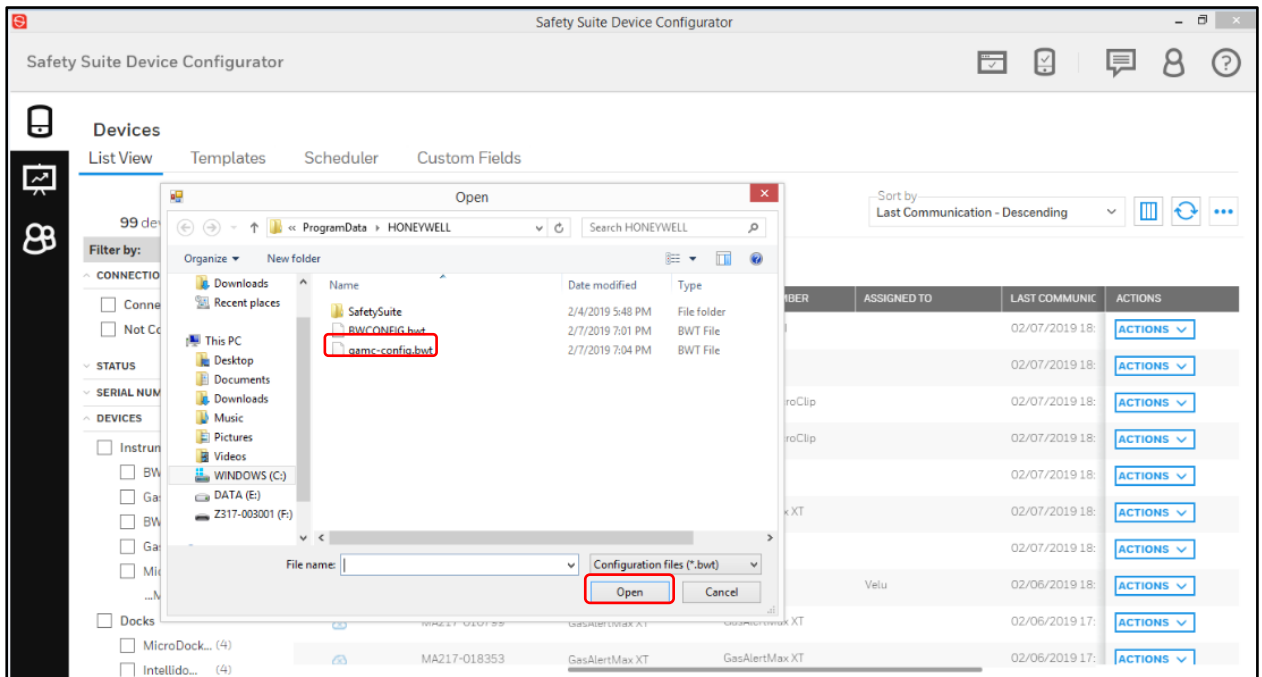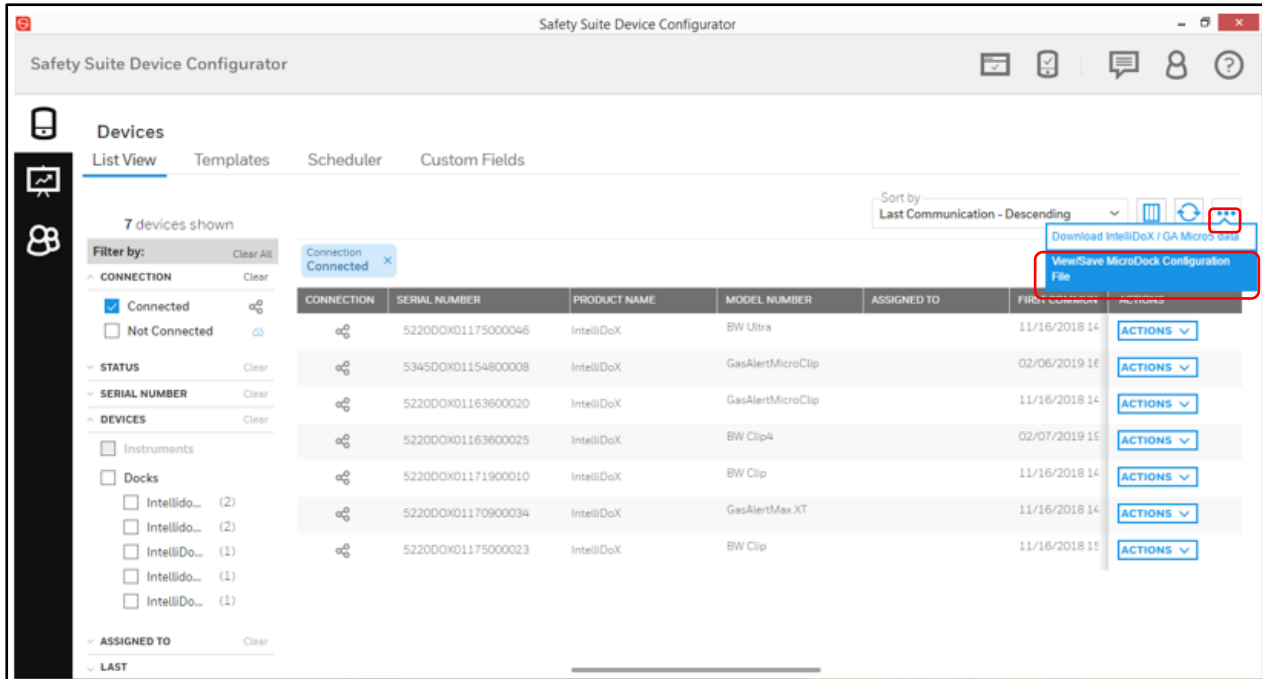

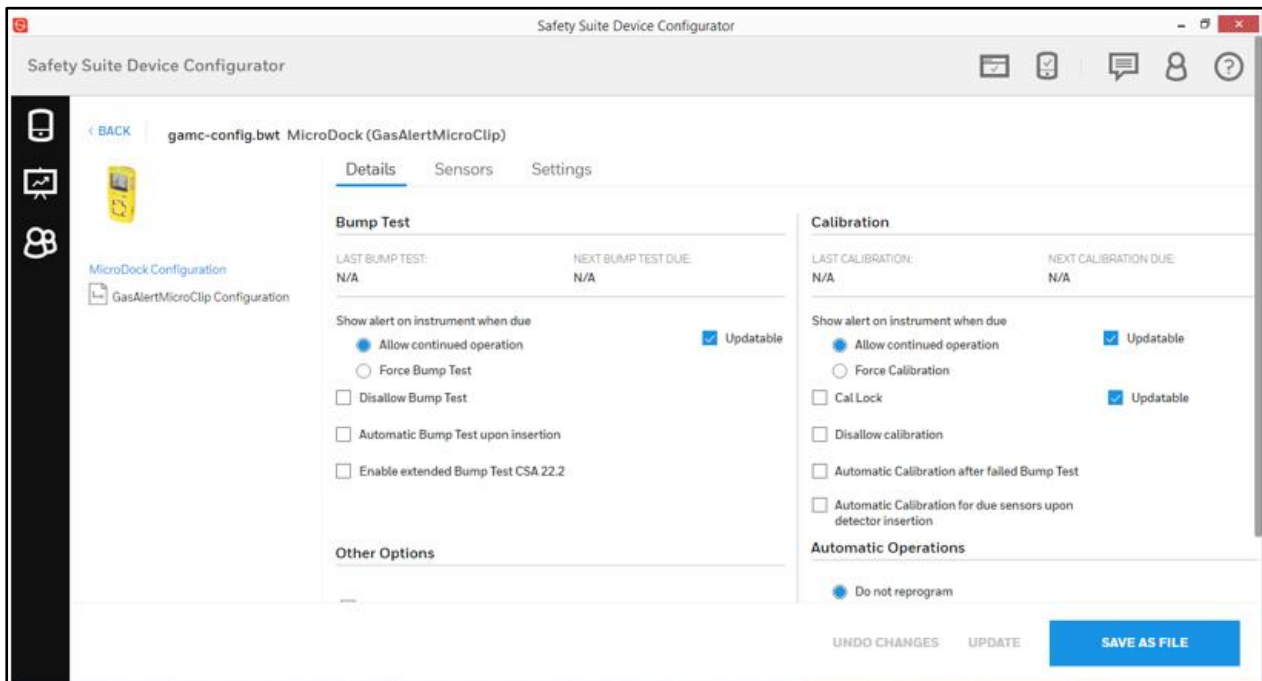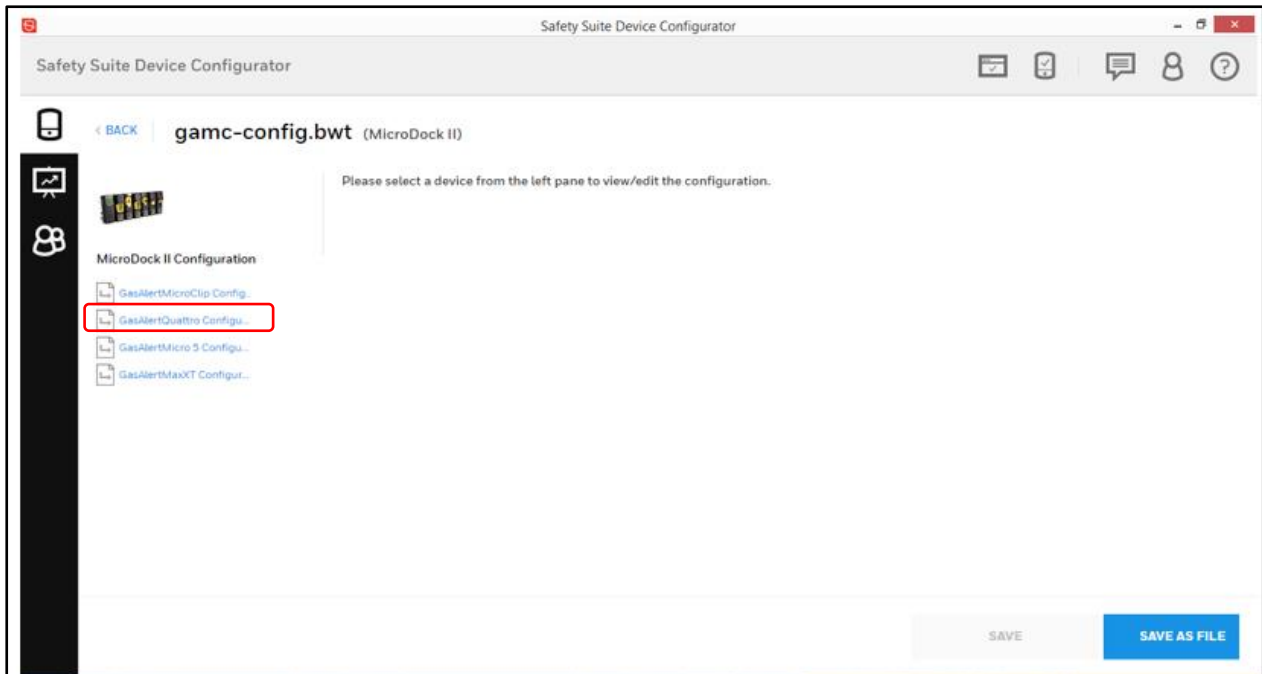

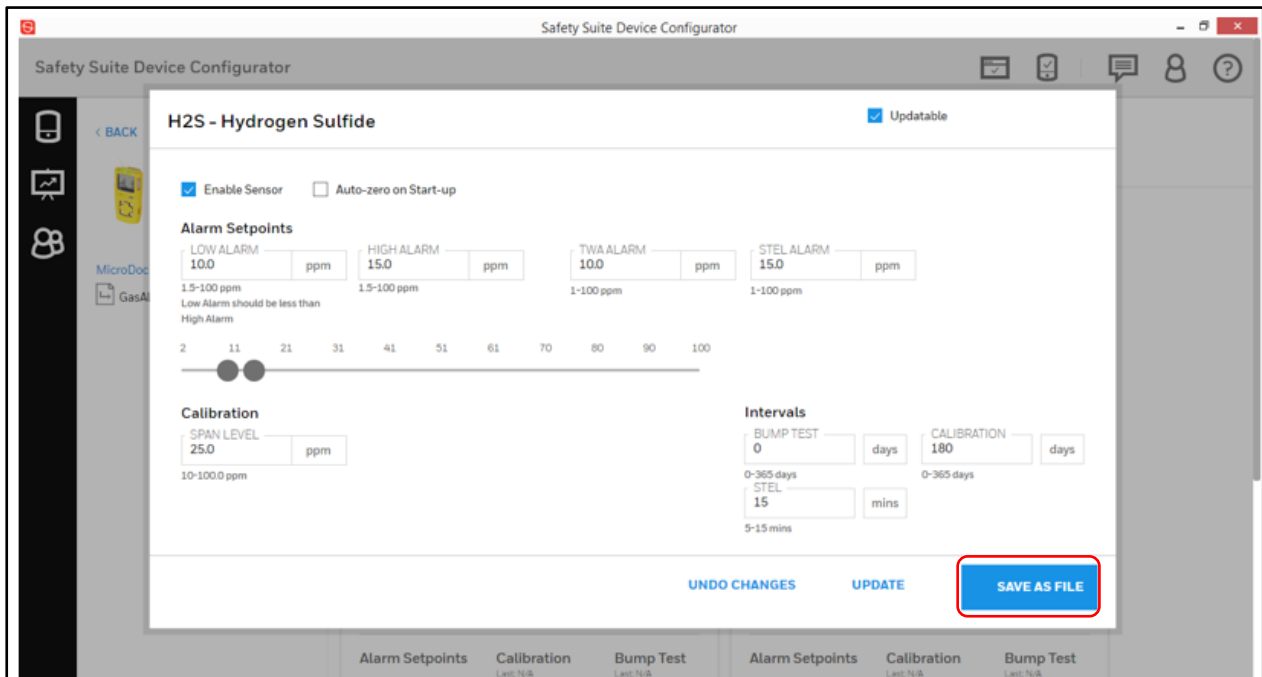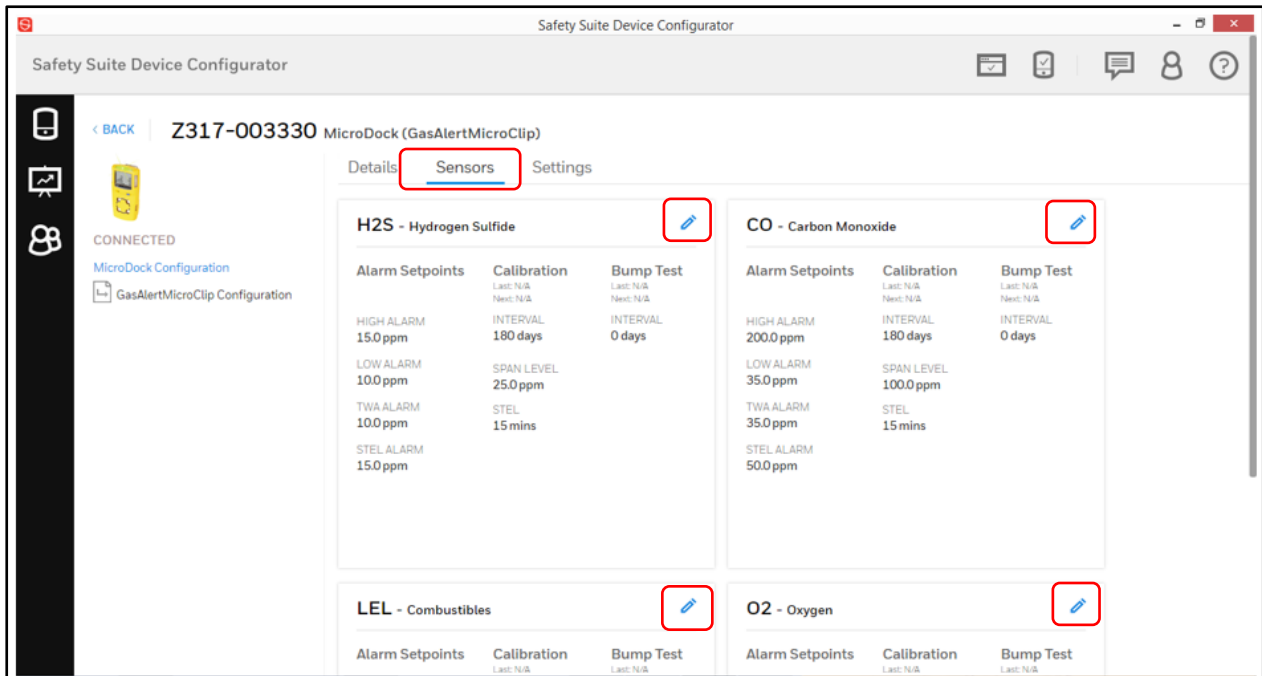

Settings can be updated across sensors and devices. Once all changes are completed the file can be saved at the user's desired location.

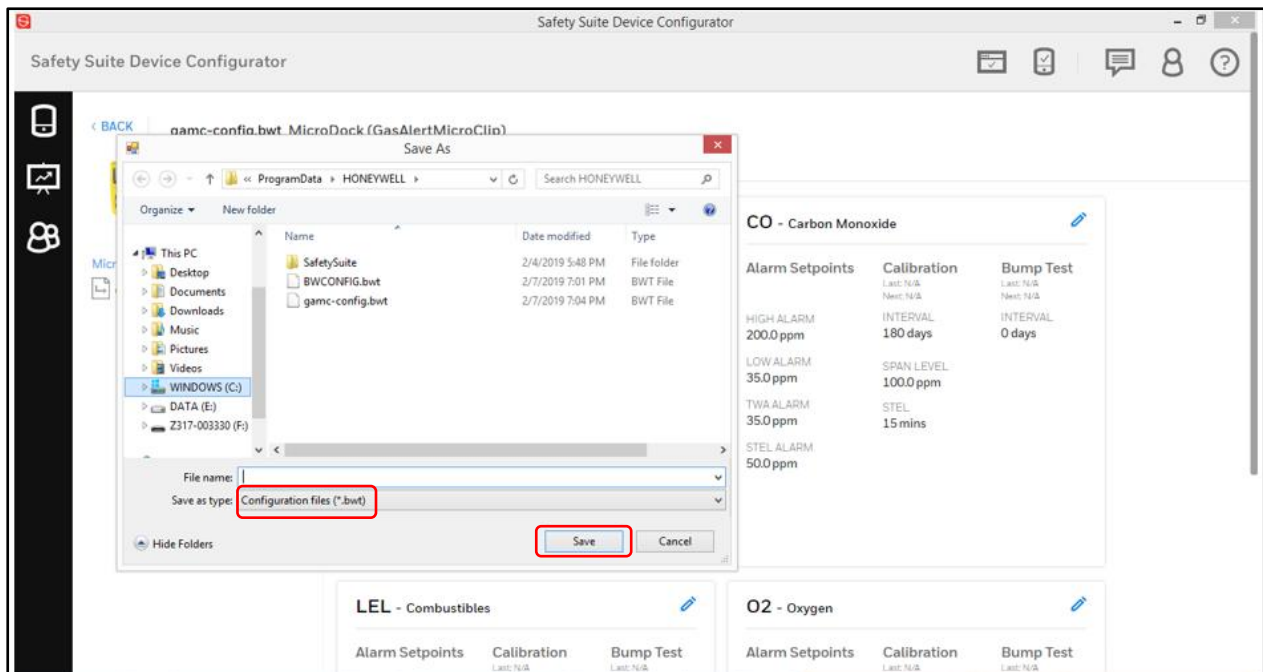

Please Note: Due to security requirements, the application may not be able to read files from certain folders. If an error is encountered, the user can retry by placing the configuration file in a different folder (ex. C:\).

Note: In order to change the device configuration in Microdock for another device type, click on the 'Microdock Configuration' link in the left hand side of the page



7 Security

The computer running Safety Suite Device Configurator should be protected from malware and external attacks. Consult your company's I.T. support or network administrator to ensure that adequate protection (anti-virus, anti-malware, secure firewall, etc.) is in place.

Note: The Safety Suite Device Configurator installer should be installed by user with Administrator Privileges. Non-administrator users should not be allowed access to the system files and folders.

7.1 Data Security

1. Make sure that the computer running Safety Suite Device Configurator is properly configured if it is used on a LAN connected to an external network. Firewalls and routers are configured to not drop required packet types (for example, ICMP, SYN). This is to prevent external users from flooding the internal network. Check with your local network administrator on how to configure the firewall and router.
2. Have the local network administrator configure the local firewall or routers to block all traffic from the RFC 1918 address space. Properly configuring boundary protection devices like firewalls or routers prevents attackers from using spoofed IP addresses that cannot be traced back.
3. Install anti-malware software on the computer.
4. Make sure any SD Card or USB memory drive connected to the machine that accesses Safety Suite software is controlled and is scanned for Malware.
5. Log out of the application after the required actions in Safety Suite Device Configurator are completed.
6. The Safety Suite Device Configurator installer/software is not decompiled or modified

7.2 Wireless Security Warning

Wireless data transmission by instruments and docking stations can extend beyond your walls and can be received by anyone with a compatible adapter. Without proper protection, data can be compromised. Use the security features of all wireless equipment in your network.

Wireless devices typically have a default name and password. You should change these to personalize them upon first installation, which decreases the potential security risk that an unauthorized user can change the configuration.

IMPORTANT!

Other Wi-Fi devices may transmit specific Wi-Fi messages that interfere with some wireless devices in a wirelessly networked system. You should not allow any untrusted Wi-Fi transmitters inside the area of location and in its proximity (approximately 50 meters).

8 Starting Safety Suite Device Configurator from the Desktop

With your computer and device connected via cable, you are ready to start communication.

1. Follow the instructions in your monitor's User's Guide. This includes turning the monitor on and making sure it is connected either directly via cable, or through a cradle that is connected to the computer via a cable. Some monitors automatically sense the computer and software, and place themselves in communication mode. Check your instruments' User's Guide for details.
2. Double-click the Safety Suite Device Configurator icon on your desktop to start the program.



3. The program starts and a login dialog box appears:


Note:

There are four access levels. The following sections cover the Administrator level, since it has the greatest functionality. For more information on roles and access levels, refer to page 31.

Type the User Name and Password, and click "OK".


9 Logging In

After your initial setup and registration procedure, you may simply login To Safety Suite Device Configurator using your Username and Password. If you wish to remain connected until you log out, click the "Keep me signed in" box. Otherwise, Safety Suite Device Configurator locks any signed-in user out of the system after 15 minutes of inactivity.

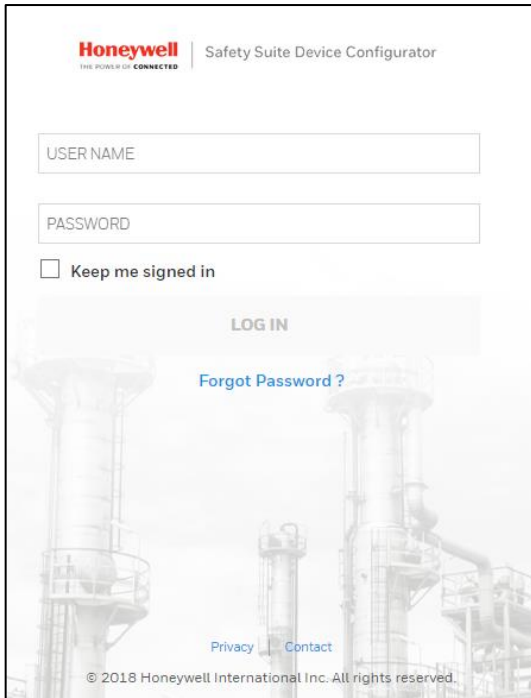

9.1 Password Recovery for Non-Administrators

If you forgot your password, click the link and follow instructions for resetting the password.

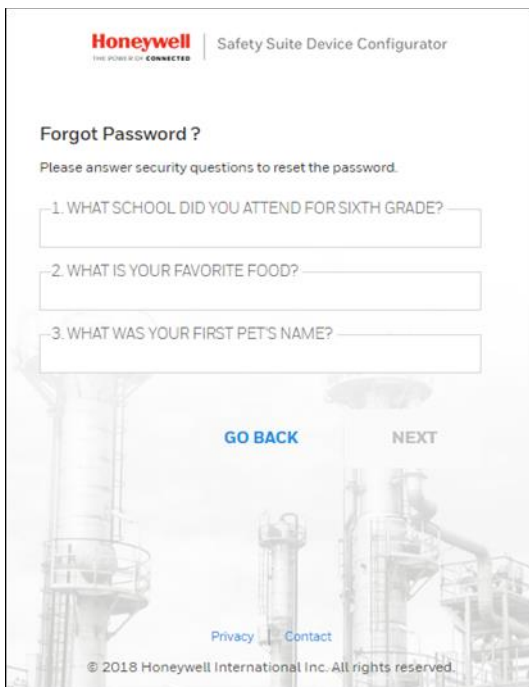


9.2 Password Recovery for Administrators

If you have Administrator access and forgot your password, follow these steps:


1. Click the “Windows” icon on the lower left side of your screen.




2. Click “All apps.”

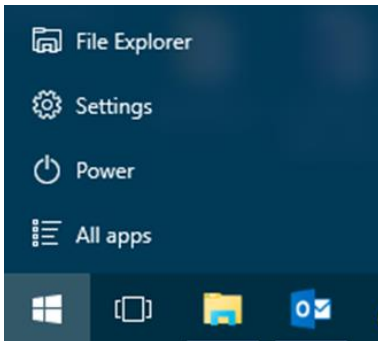

3. Scroll down until you see “Honeywell.” Click the downward arrow to see “Unlock Administrator Account.”

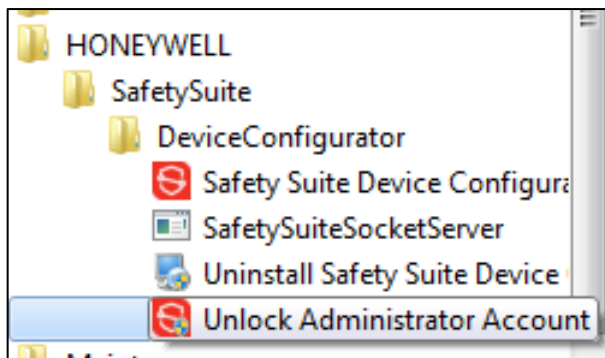


4. When the “Windows Security” window appears, type in your Administrator password for the PC.

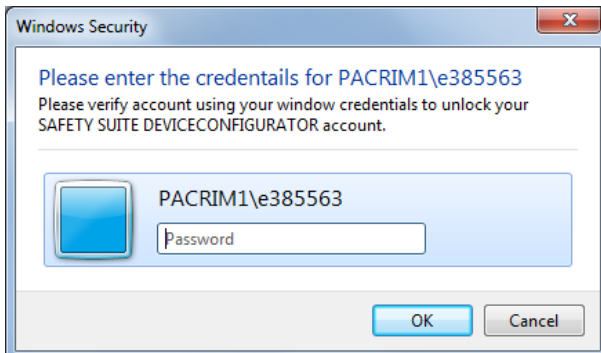


5. Click “OK.” An activation code is shown.
6. Use this activation code to login to Safety Suite Device Configurator.

9.3 Password expiry.

The expiry date for each password is 90 days from the day it is set or changed, When your password approaches the expiry date (85 – 90th day), a warning pop up will appear on the screen to remind you to change the password.

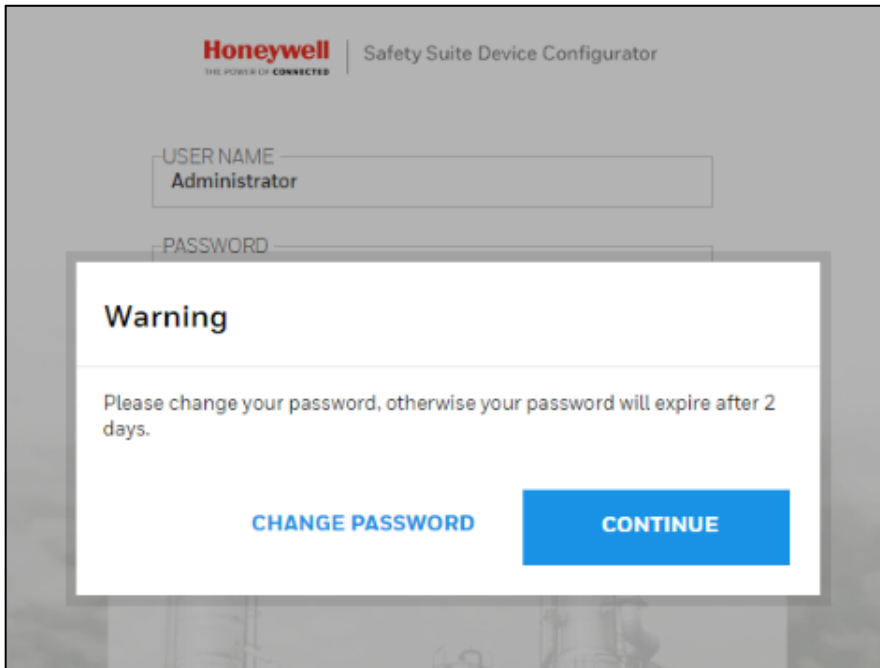

Click on “CHANGE PASSWORD” and change your password.

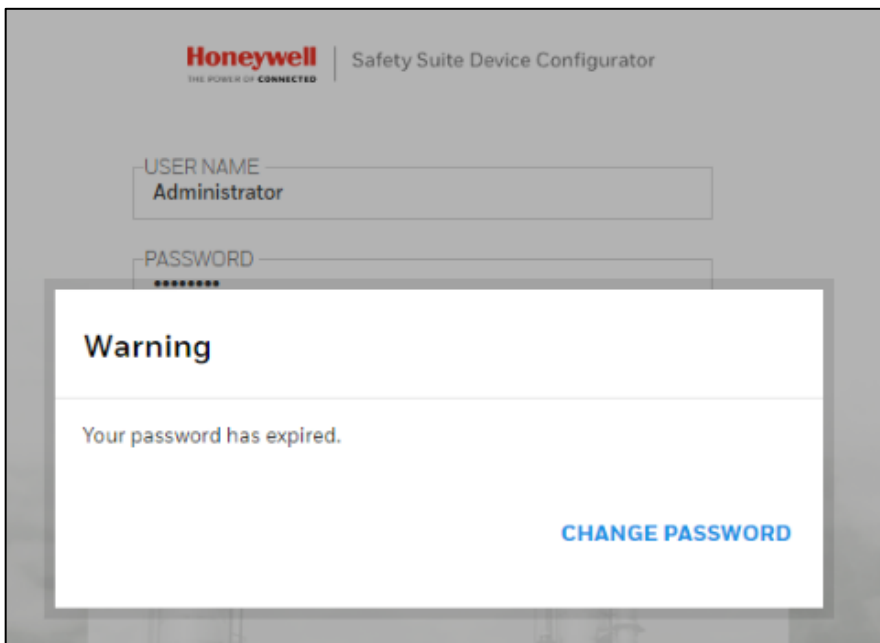

If your password expired, then click on “CHANGE PASSWORD” and answer the security questions.

Honeywell | Safety Suite Device Configurator
THE POWER OF CONNECTED

Forgot Password ?
Please answer security questions to reset the password.

1. WHAT WAS YOUR FIRST PET'S NAME?

2. WHAT IS YOUR FAVORITE FOOD?


3. WHAT WAS YOUR CHILDHOOD NICKNAME?

[GO BACK](#) [NEXT](#)

[Privacy](#) | [Contact](#)

© 2019 Honeywell International Inc. All rights reserved.

Answer all the Security questions and click on NEXT, A Change Password screen will appear to let you create a new password.

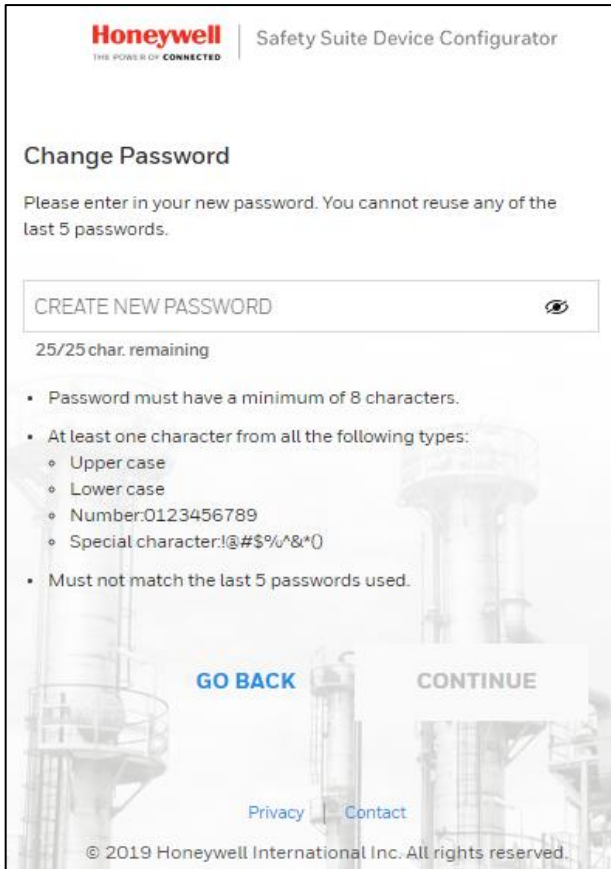


9.4 Login Process

During login, Safety Suite Device Configurator checks whether you have registered your software. If it has not been registered, then this window appears to prompt you. You can fill in the fields and click “Register” to send your registration.

The main screen is shown in its default state, with Devices selected in List View.

Note:

You may not see the list until you have used the Settings page.

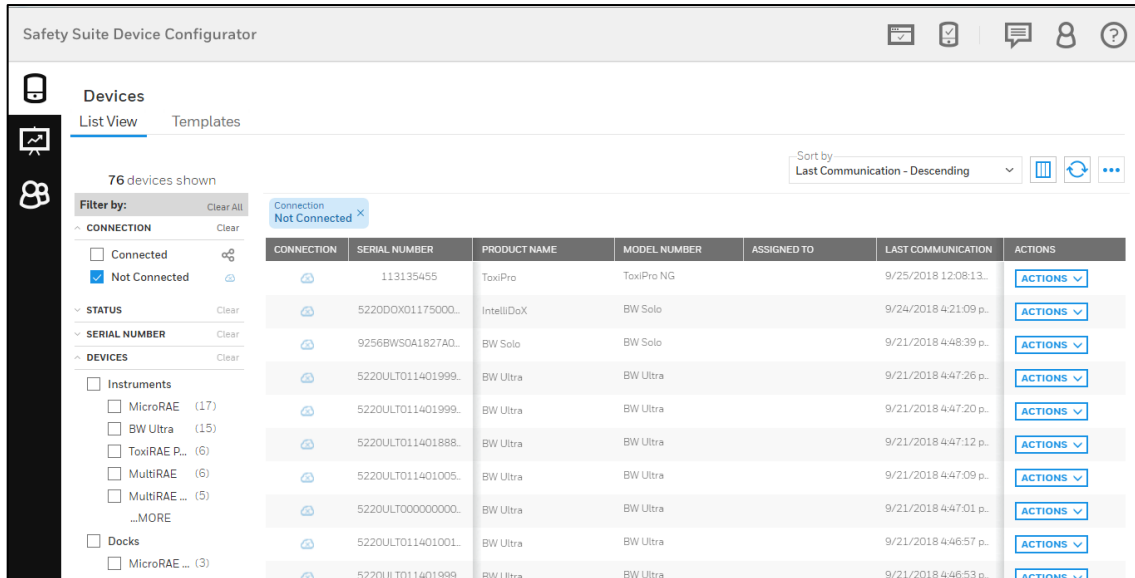

For details on navigating and using Safety Suite Device Configurator features, click the “Help” button at the upper right corner of the screen.

10 Title Bar/Quick-Access Toolbar

The Title Bar/Quick-Access Toolbar is always visible. It acts as an information “dashboard” to give insight into important functions, regardless of which view is being used.



10.1 Registrations

If all software or application registrations are up to date, then no number is shown. If a number is shown, it indicates how many registrations need to be updated. To view registrations that need updating, click the icon.



10.2 Devices

If all device registrations are up to date, then no number is shown. If a number is shown, it indicates how many devices need their registration updated. To view registrations that need updating, click the icon.

Note: If your software has not been registered, you must register it before you can view device registrations.




10.3 Download Status


Download Status shows whether updates are being downloaded. If a number is shown, it indicates the number of downloads pending. If there is no number and you click on the icon, a message says, “No download in progress”.




If a number is shown, click on the icon for details:

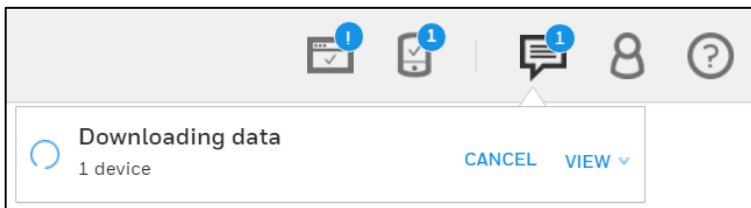

For more information, click “VIEW”:

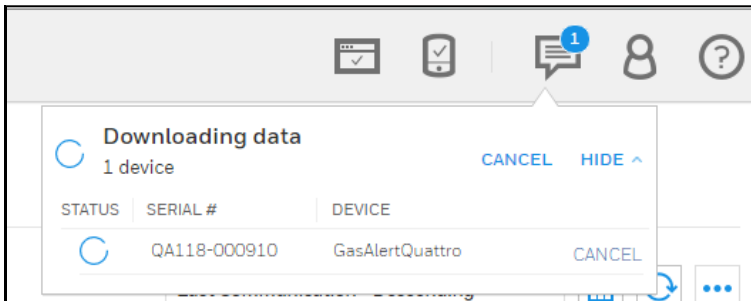

If no download is in progress, there is no number on the icon, and if you click it, this message is shown:

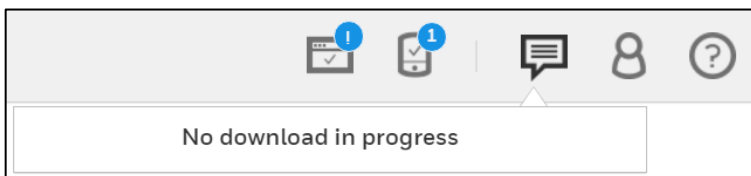


Note: When a download is in progress, performing an action with a device will not work. However, you can perform other activities.

10.4 Role Information

Role Information provides insight and management of the current logged-in user’s role and settings.



Click the icon to view the role's name, as well as to Edit Profile, Sign Out, review/change Settings, or view the User Role List.

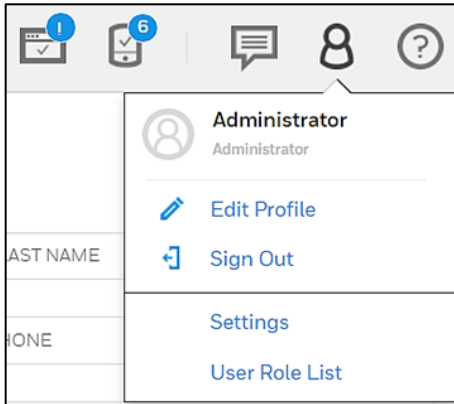

10.4.1 Role Name

The Role Name tells you the role of the person logged in. Default values include Standard User, Advanced User, Administrator, and Worker. Each user must be assigned one or more roles. Click the appropriate box or boxes.





10.4.1.1 Role Names and Access Levels

The following definitions explain the four roles and their access:

- Administrator – Access to all the features of the application
- Advanced User – Access to all Device Management features and Reporting, except User Management
- Standard User – Access to Data Download, Device History and Reporting.
- Worker – No access to any software features, only what are defined in the system for tracking worker device assignments

10.4.2 Edit Profile

The profile includes details about the role/person currently logged in. Details can be viewed and changed.

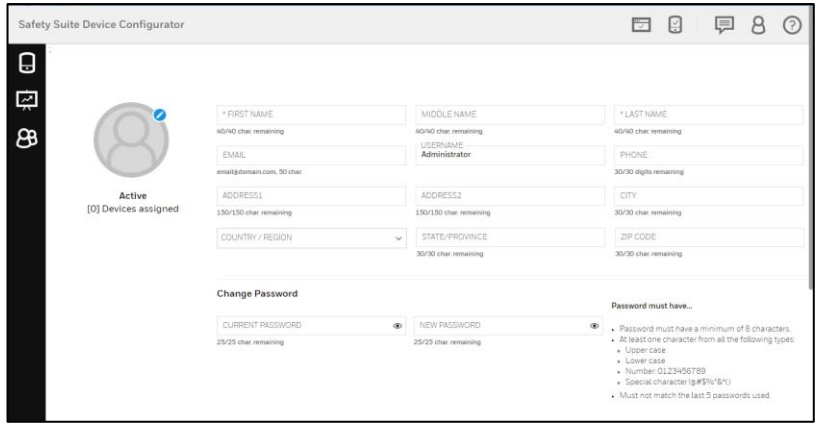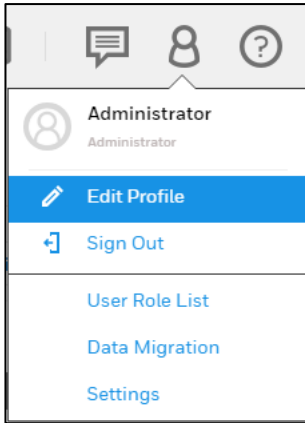


10.4.2.1 Update Profile Picture


Click the icon to open the dialog for uploading an image for the profile. The image can be either a .jpg or .png file, but it must be less than 1MB.

To upload an image:

1. Click the blue button.

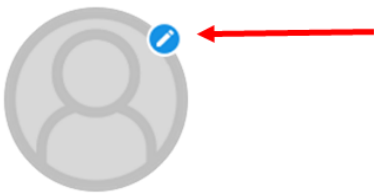

2. Click "Upload Photo."
3. Locate an image on your computer and select it.
4. Click "Open."

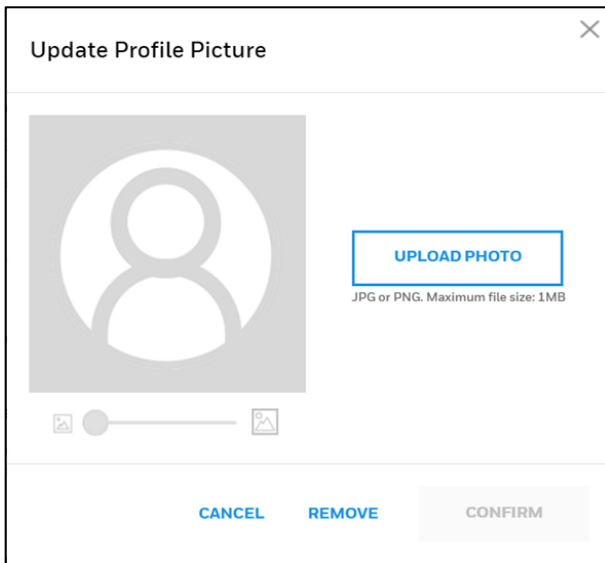

5. When the image appears, move it around with your mouse and/or change its size by adjusting with the slide control.

6. When you are satisfied, click “Confirm”.

Note:

Click “Cancel” if you decide not to change the picture, or “Remove” to remove an existing picture.

10.4.2.2 Personal Information

View the personal information attached to this role. All aspects can be changed except the username.

10.4.2.3 Change Password

You can change the password. You must supply the current password and then type the new password. The password must follow these rules:

- The password must have a minimum of 8 characters.
- The password must include at least one character from all the following types:
 - UPPERCASE
 - lowercase
 - Number: 0 1 2 3 4 5 6 7 8 9
 - Special character, including: ! @ # \$ % ^ * ()
- The new password must not match any of the last five passwords that have been used.

10.4.2.4 Update Security Questions

In case you forget your password and want to reset it, you will have to answer security questions. Here is where you put the answers that must be matched if you want to regain access after forgetting your password.


1. Select a security question from each pull-down list.
2. Type in an answer for each of the questions.
3. Click “Update.”

10.4.3 Sign Out

Click here to sign out.

Note:

If you sign out, you will have to sign in again for access to Safety Suite Device Configurator.

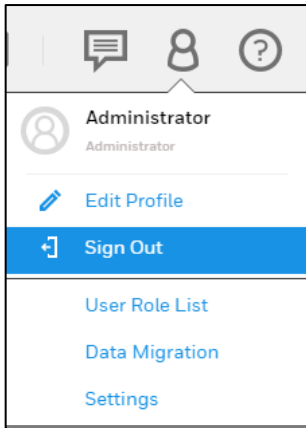


10.4.4 Settings

System Settings is an overview of the System Name, IP Address, MAC Address, and Software Version. It also lists Product Services and Service Ports.

Note:


After you make changes to settings, you must go back to the Device list and select “Manual Refresh.”

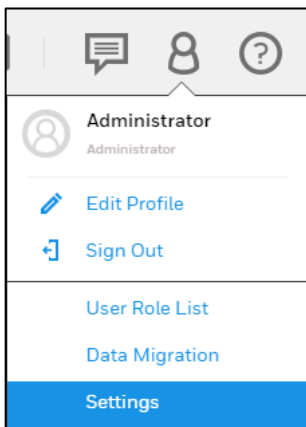

- Click “Save” to save any changes you make.
- Click “Undo Changes” to undo them.
- Click “Restore Defaults” to clear all changed values and revert to default values that are supplied with the software.

Note:

If you choose to restore default values, your customized settings are deleted and cannot be retrieved.

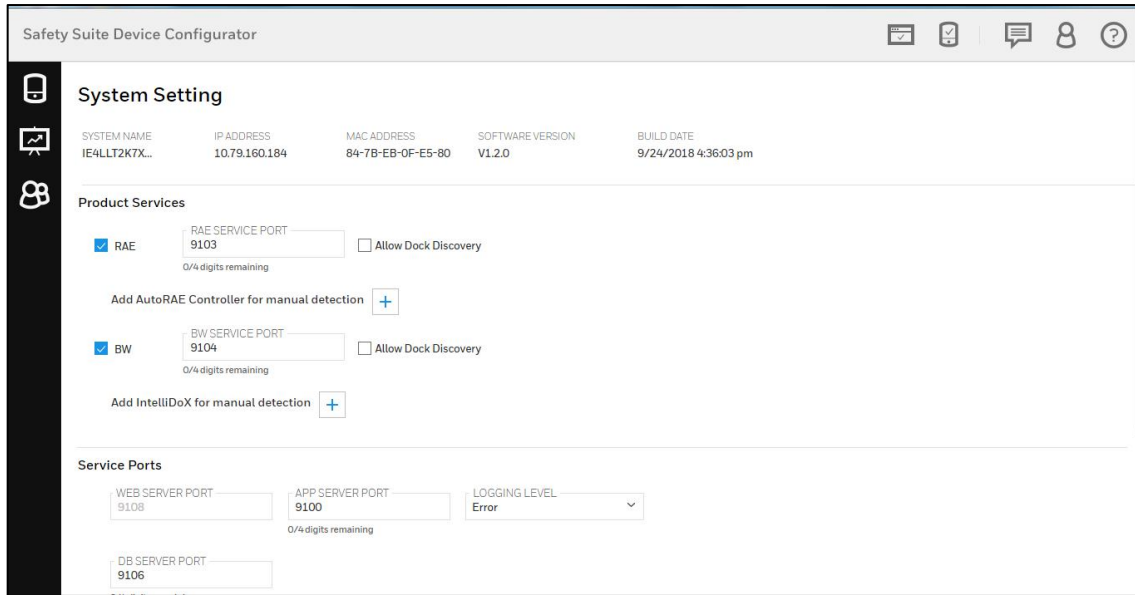


10.4.4.1 Product Services

Services for RAE Systems instruments and BW instruments are separately shown, and include the currently used ports. If docking stations are included on the network, you can check “Allow Dock Discovery” so that as docks are included, they are part of the roster.

Note:

Each service can be turned on or off by checking or unchecking the box labeled RAE or BW.

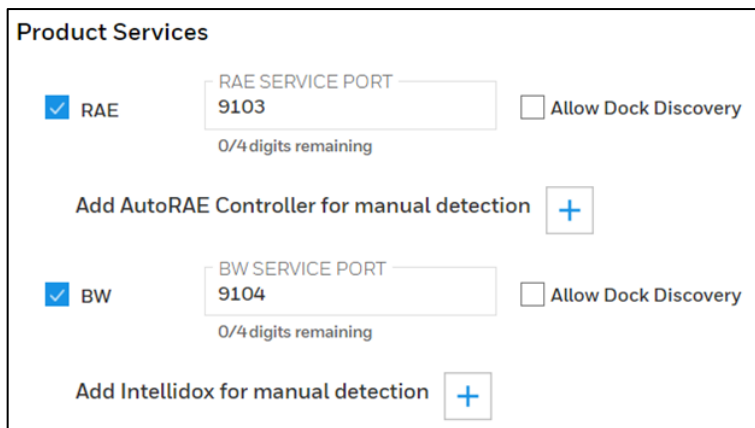

You can manually add an AutoRAE Controller or IntelliDoX: Click the “+”, and there are fields for IP Address and Port number. If you decide to remove a manual selection, click the “trash” icon.

Product Services

RAE Allow Dock Discovery
0/4 digits remaining

Add AutoRAE Controller for manual detection

xxx.xxx.xxx.xxx 4/4 digits remaining

10.4.4.2 Service Ports

View/change settings for Service Ports, including Web Server Port, Application Server Port, and Database Server Port.

Service Ports

0/4 digits remaining

0/4 digits remaining



10.4.4.3 Local Settings

Local Settings include Measurement Units.

Local Settings

10.4.5 User Role List

Click “Standard User,” “Advanced User,” “Administrator,” or “Worker” to see which access to functions are available for that role.

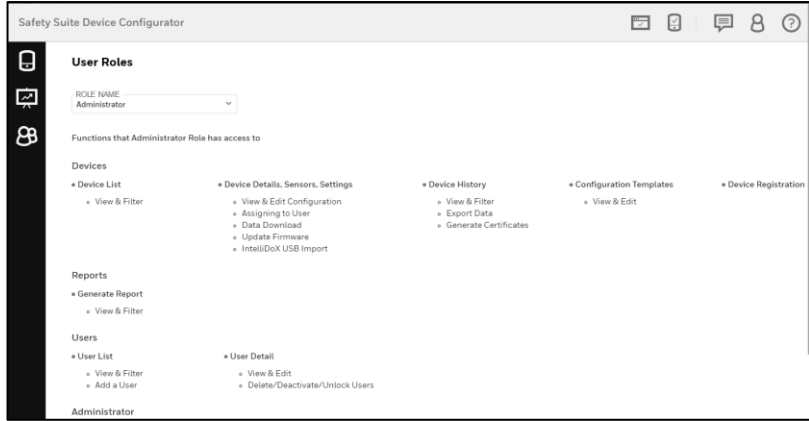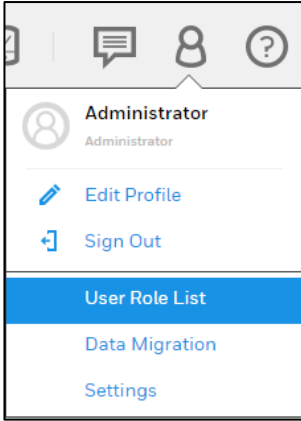

10.5 Help



Click this button for Help documentation.

11 Views

Safety Suite Device Configurator has two primary screens: Devices and User List.

- **Devices** provides insight based on the devices in use.
- **User List** focuses on the users and the devices assigned to or associated with.



Devices view






Generate Report view




User List view

Here is the hierarchy of functions in Safety Suite Device Configurator:

 Devices	
List View Filter by: Connection Status Serial Number Devices Assigned To Last Communication First Communication Actions: Device Details Device History Archive Device	Templates Filter By: Product Templates Actions: Edit Delete
 Generate Report	
 User List	
Filter by: Status Name Device Assigned User Role Username Actions: User Details	

11.1 Devices

When you select “Devices,” the main screen is shown with Devices selected, in the List View.

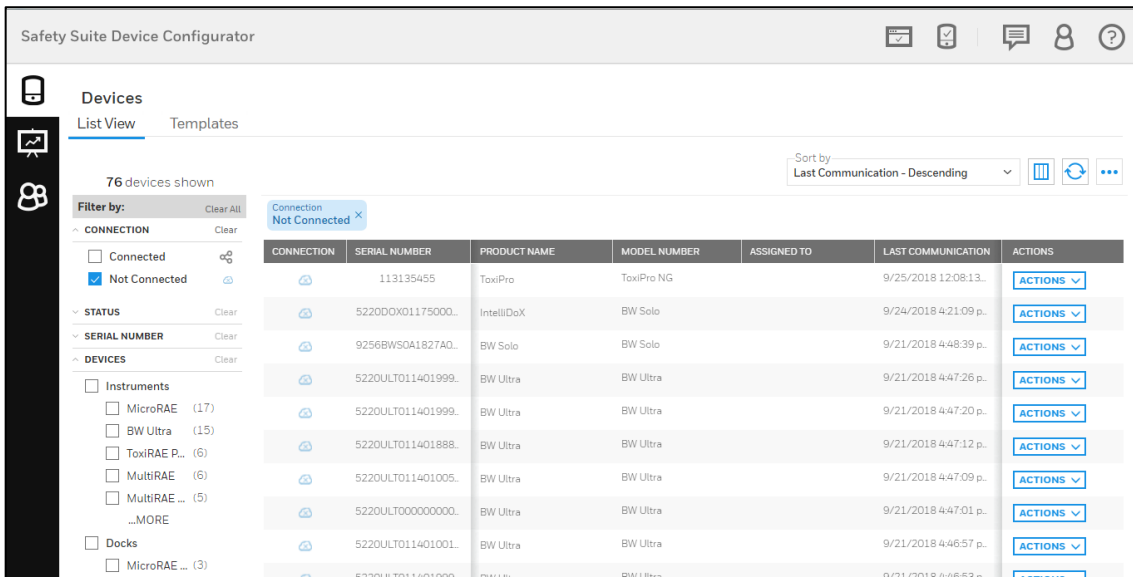

The screenshot displays the 'Safety Suite Device Configurator' interface. The 'Devices' section is active, showing a list of 76 devices. The interface includes a sidebar with navigation icons, a filter menu, and a table of device details.

Filter by: Clear All

- Connected
- Not Connected

STATUS Clear

SERIAL NUMBER Clear

DEVICES Clear

- Instruments
 - MicroRAE (17)
 - BW Ultra (15)
 - ToxiRAE P... (6)
 - MultiRAE (6)
 - MultiRAE ... (5)
 - ...MORE
- Docks
 - MicroRAE ... (3)

Table:


CONNECTION	SERIAL NUMBER	PRODUCT NAME	MODEL NUMBER	ASSIGNED TO	LAST COMMUNICATION	ACTIONS
	113135455	ToxiPro	ToxiPro NG		9/25/2018 12:08:13 p.	ACTIONS
	5220DOX01175000...	IntelliDoX	BW Solo		9/24/2018 4:21:09 p.	ACTIONS
	9256BWS041827A0...	BW Solo	BW Solo		9/21/2018 4:48:39 p.	ACTIONS
	5220ULT011401999...	BW Ultra	BW Ultra		9/21/2018 4:47:26 p.	ACTIONS
	5220ULT011401999...	BW Ultra	BW Ultra		9/21/2018 4:47:20 p.	ACTIONS
	5220ULT011401888...	BW Ultra	BW Ultra		9/21/2018 4:47:12 p.	ACTIONS
	5220ULT011401005...	BW Ultra	BW Ultra		9/21/2018 4:47:09 p.	ACTIONS
	5220ULT0000000000...	BW Ultra	BW Ultra		9/21/2018 4:47:01 p.	ACTIONS
	5220ULT011401001...	BW Ultra	BW Ultra		9/21/2018 4:46:57 p.	ACTIONS
	5220ULT011401999...	BW Ultra	BW Ultra		9/21/2018 4:46:53 p.	ACTIONS

11.1.1 Device Hierarchy


The relationship of instruments to docking stations and their controllers is shown under “Product Name.”

Note:

This “parent/child” hierarchy is reflected in the “Filter by” section.

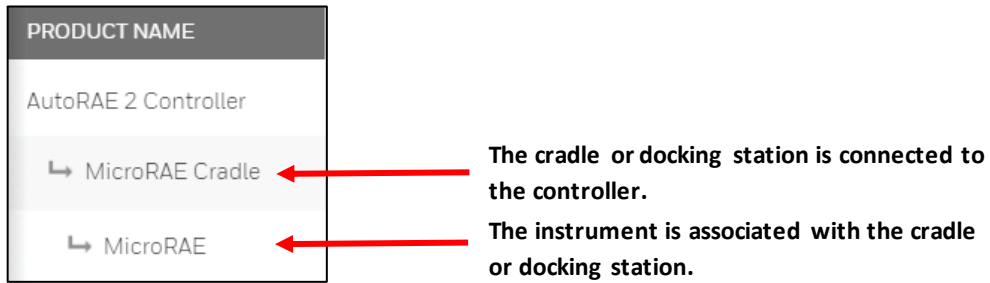


If a controller is connected to multiple docks or cradles, and if there are multiple instruments, the hierarchy is extended to reflect the relationships.

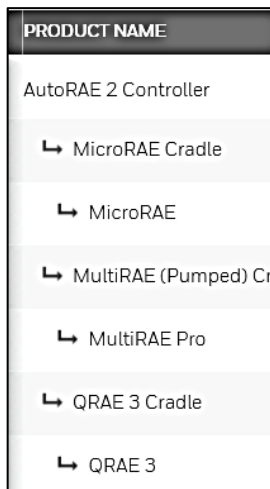

Instruments that are not associated with a docking station or controller are simply shown as individual list items.


11.1.2 Sorting and Organization

At the top of the screen, along the right side, are controls for sorting and organization:



11.1.2.1 Sort by

Click “Sort by” to change the sort order of the list for quickest reference:

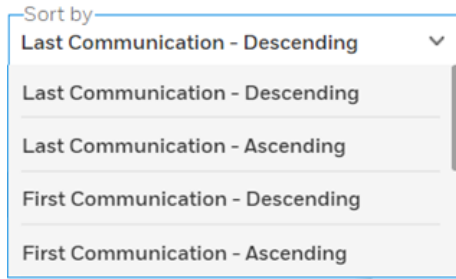


Depending on which columns are shown, the options change in the pull-down menu. Select from the list and then click on your choice. The sort order changes to reflect your selection.

11.1.2.2 Columns

Click “Columns” to open a menu where you can select columns you want to appear on the screen:



A check mark in a box indicates that you have selected this column to be shown. Boxes/names in light gray indicate that their visibility cannot be changed.

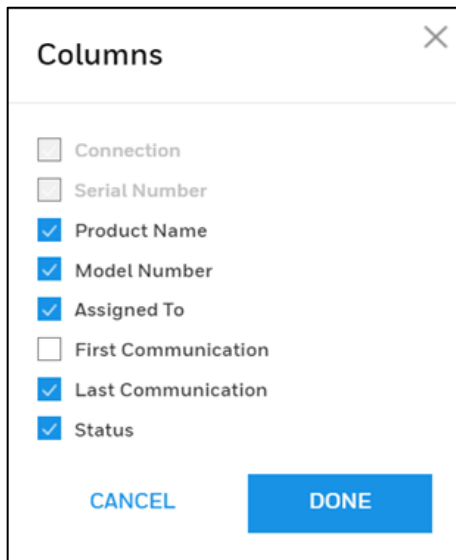

11.1.2.3 Refresh

Click Refresh to update the information on the screen. It is important to do this whenever you connect a new device to the computer running Safety Suite Device Configurator.





Refresh

11.1.2.4 List View

When the list of instruments is shown, you can manage it in a variety of ways using filters.

At the top, the total number of devices shown is indicated. Also indicated is the number of filters, shown by filter category.

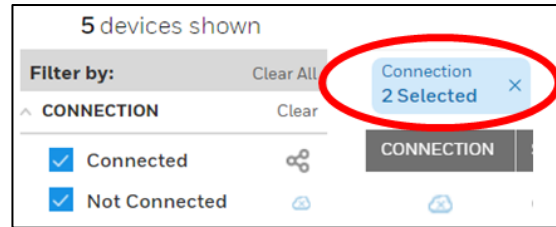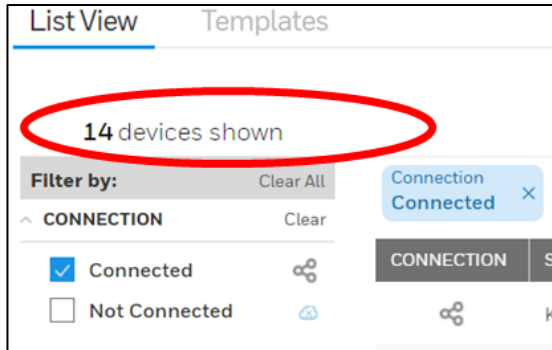


12 Assign Device to Worker

Device view allows you to assign the device to the worker, the device only assigns with the user which has Worker Role defined, for more information about defining Roles refer section [Role Name](#).

To Assign the device to a worker.


1. Go to the “Device” from main screen menu.
2. Switch to “List View” and “Clear Filter” to view all devices

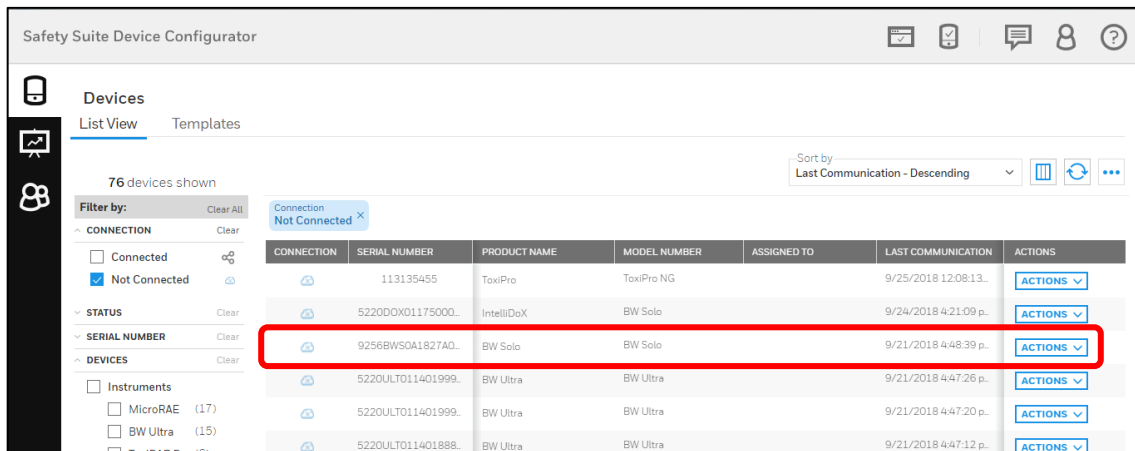

3. Select the Device that needs to be assign to the worker.
4. Click on the “Action” dropdown list and select “Device Details”.



5. Select the registered Worker's Name from Assignment dropdown list.

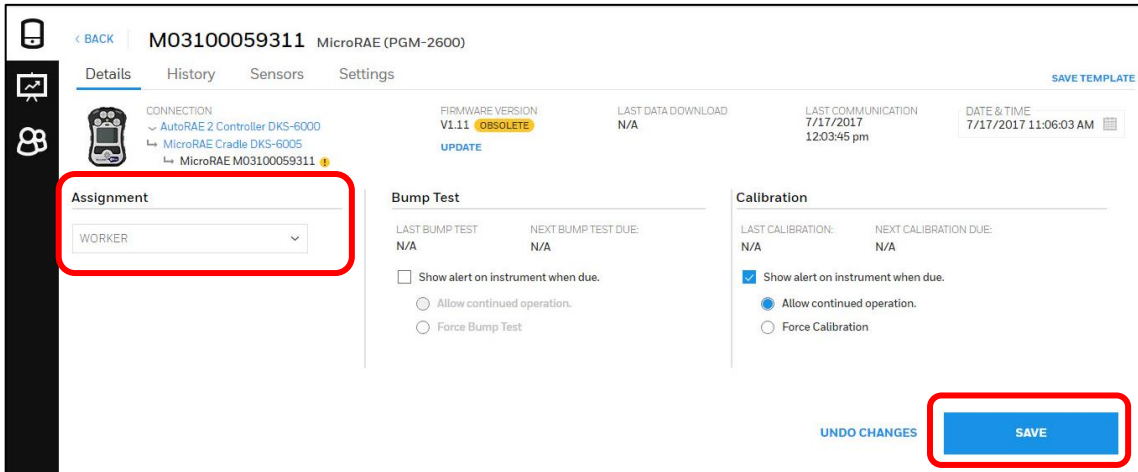

6. Click on “Save” to changed Settings.

Note: Multiple device can be assign to a single worker, but single device cannot be assigned to more than one person.


13 Filter by

Several filters are included so that you can expand or pare down the data. This is especially valuable when you are managing many instruments.

Filters include:

- Connection
- Status
- Serial Number
- Devices
- Assigned To
- Last Communication
- First Communication

As filters are selected, they are shown above the list, and the list updates to reflect your choices. You can remove a filter directly in the “Filter by” menu or by clicking the “x” in a filter shown above the list.

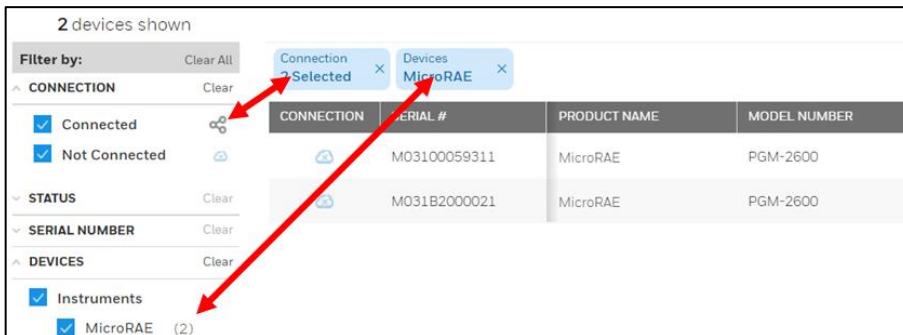

13.1 Connection


Click “Connected” or “Not Connected,” or both to include instruments that are connected to the PC running Safety Suite Device Configurator and those in the roster that are not connected.

Status

Click “Archived” to see any instruments that are archived.


Serial Number

Search for devices by serial number. Type in the serial number of a device in the roster, or select from the list that appears when you start typing or mouse over the box.

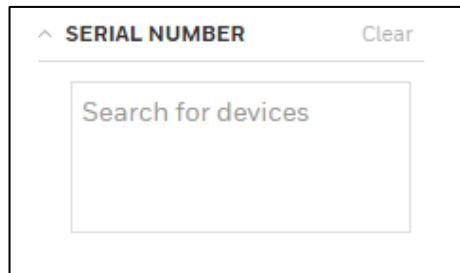

^ SERIAL NUMBER Clear

Search for devices

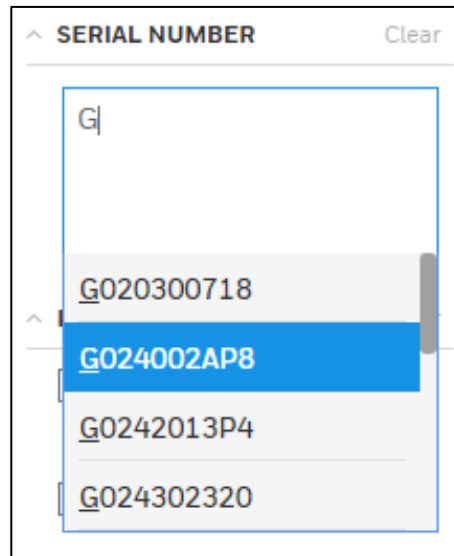


^ SERIAL NUMBER Clear


G|

- G020300718
- G024002AP8**
- G0242013P4
- G024302320



Your choice is shown in the box.

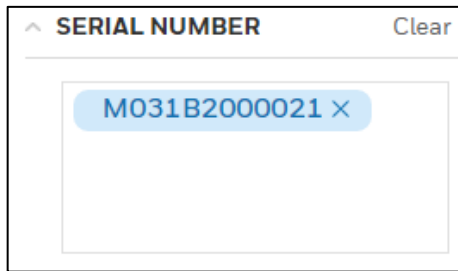

You can select multiple serial numbers, too:

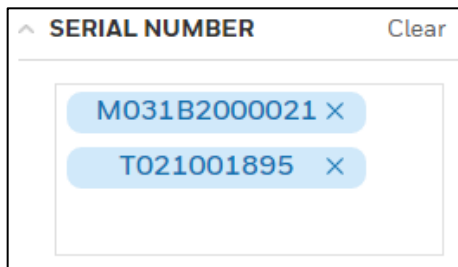


Your choice is shown in the list, along with indication of how many devices are shown:

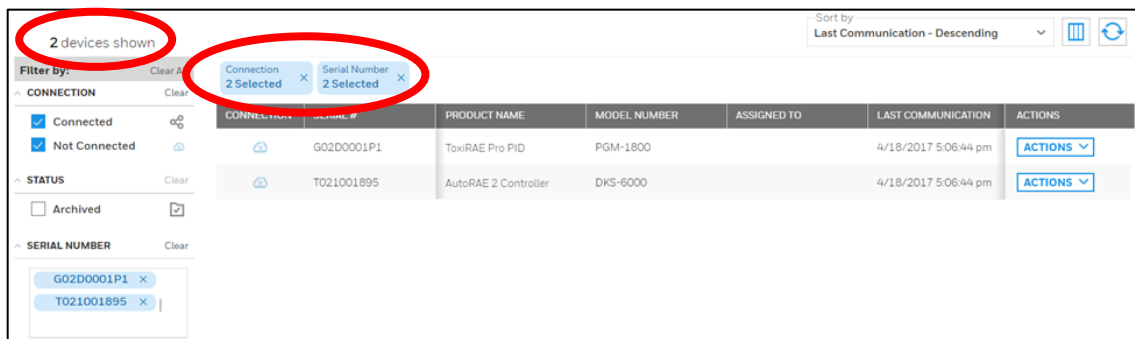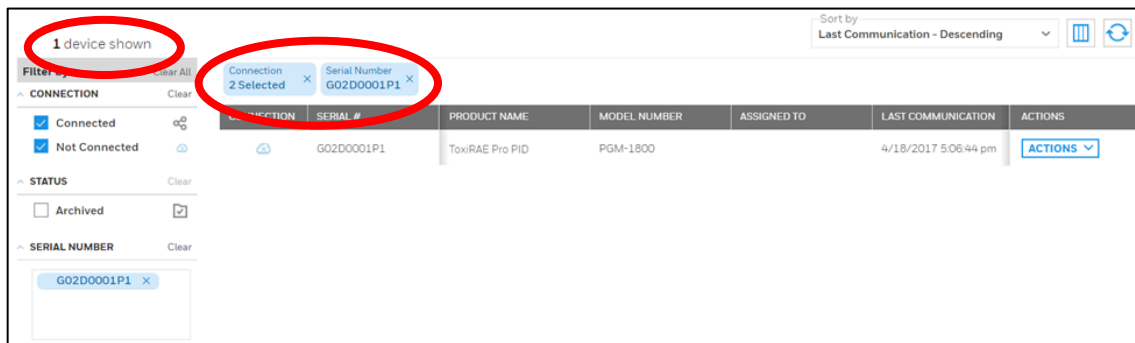

You can clear all the selections by clicking "Clear" or you can select which ones you want to clear by clicking on the "X" in an individual tag.


13.2 Devices

Two choices of devices are available: Instruments and Docks. You can select all instruments or all docks (docking stations) by clicking Instruments or Docks, respectively. In addition, individual instruments or docks can be selected or deselected.

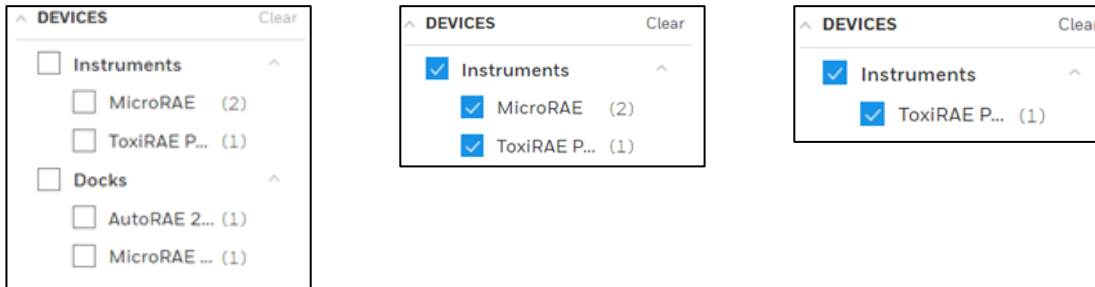


13.3 Assigned To

If you want to filter by who an instrument is assigned to, type a name in the box or use the pull-down menu to select a name. You can clear a person's name and associated information by clicking "Clear."

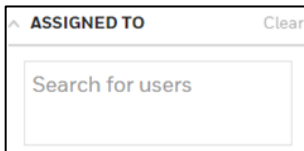

13.4 Last Communication

You can search for an instrument by setting a date range for filtering by its last communication. Click on the "FROM" calendar, select a date, and then click on the "TO" calendar and select a date.

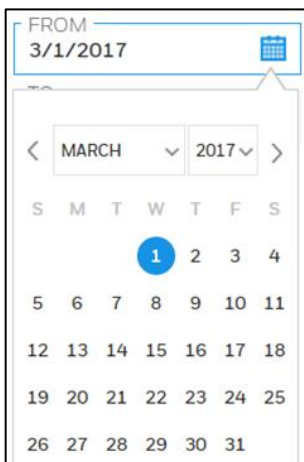

This sets your date range for the last communication.



^ LAST COMMUNICATION Clear


FROM 3/1/2017

TO 5/9/2017

Click "Clear" to clear the selected "TO" and "FROM" dates.

13.5 First Communication

You can search for an instrument by setting a date range for filtering by its first communication. Click on the "FROM" calendar, select a date, and then click on the "TO" calendar and select a date.

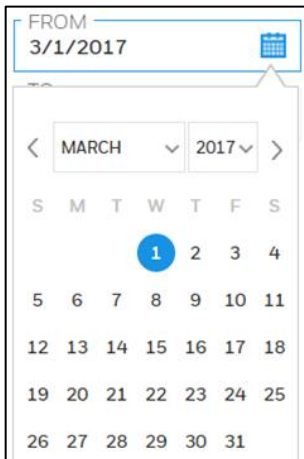

FROM 3/1/2017

< MARCH 2017 >

S M T W T F S

1 2 3 4

5 6 7 8 9 10 11

12 13 14 15 16 17 18

19 20 21 22 23 24 25

26 27 28 29 30 31

This sets your date range for the first communication.



^ FIRST COMMUNICATION Clear

FROM 1/5/2017

TO 5/9/2017

Click "Clear" to clear the selected "TO" and "FROM" dates.

13.6 Actions

Actions consist of things you can do with each device's data.



13.6.1 View the list of Devices


User can view the list of devices connected as per connection, serial number, product name, model number, assigned to, first communication, last communication, and status of device in both Offline and Online mode in Device Configurator under **Devices, List View**.

User can also apply filter, sort, and add custom fields column to the grid.

The screenshot shows the 'Safety Suite Device Configurator' interface. The main content area displays a table of devices with the following columns: CONNECTION, SERIAL NUMBER, PRODUCT NAME, MODEL NUMBER, ASSIGNED TO, FIRST COMMUN, and ACTIONS. There are 4 devices shown. The 'Connection' filter is set to '2 Selected'. The table data is as follows:

CONNECTION	SERIAL NUMBER	PRODUCT NAME	MODEL NUMBER	ASSIGNED TO	FIRST COMMUN	ACTIONS
	5220ULT01181700095	BW Ultra	BW Ultra		01/30/2019 1E	ACTIONS
	M03100084611	MicroRAE	PGM-2601		01/30/2019 14	ACTIONS
	M03100083111	MicroRAE	PGM-2602		01/25/2019 1E	ACTIONS
	M03100084511	MicroRAE	PGM-2601		01/21/2019 1E	ACTIONS


In List View user can also view the device details, device history, and also archive the device under Actions tab.

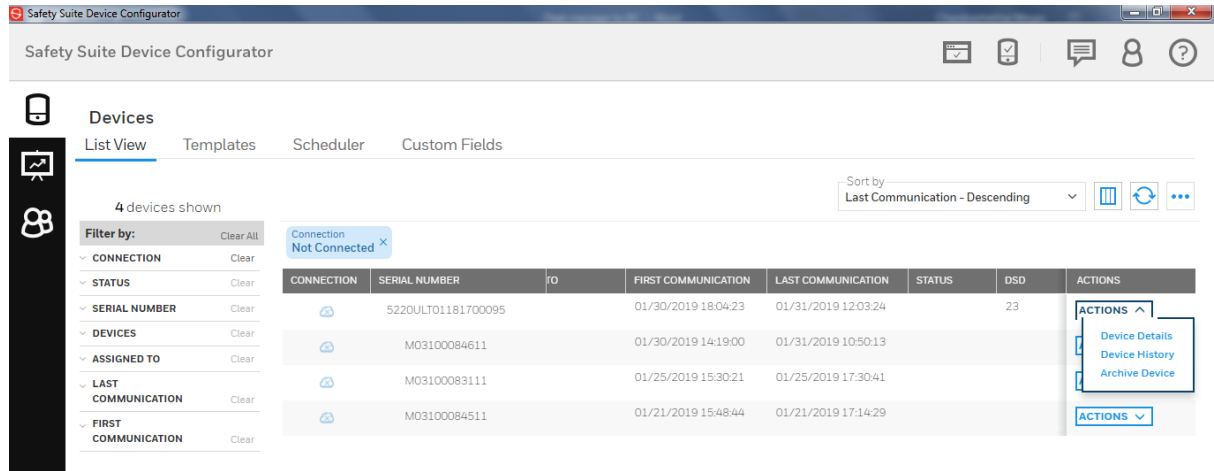


13.6.2 Device Details

Device Details include details of the device, including history, installed sensors, and settings.

To view the device details in Devices, List View click on ACTIONS drop down list, then click on **Device Details**.

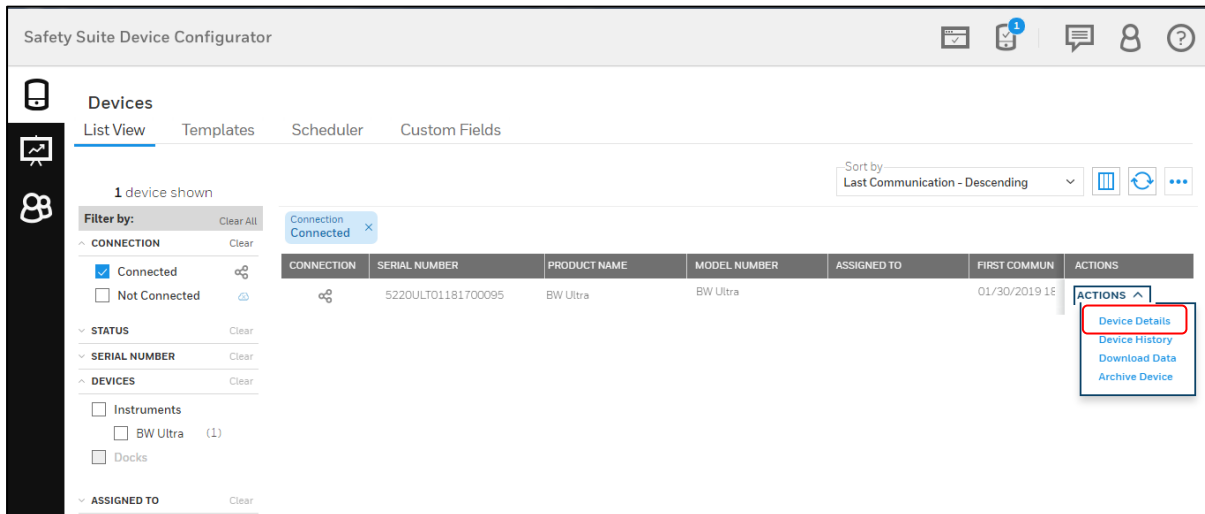


In device details user can view and edit fields such as, last data download and last communication mm/dd/yy and time. View current Firmware Version of the device or update latest version if available, Unassign worker, view or schedule Bump Test and Calibration of the device.

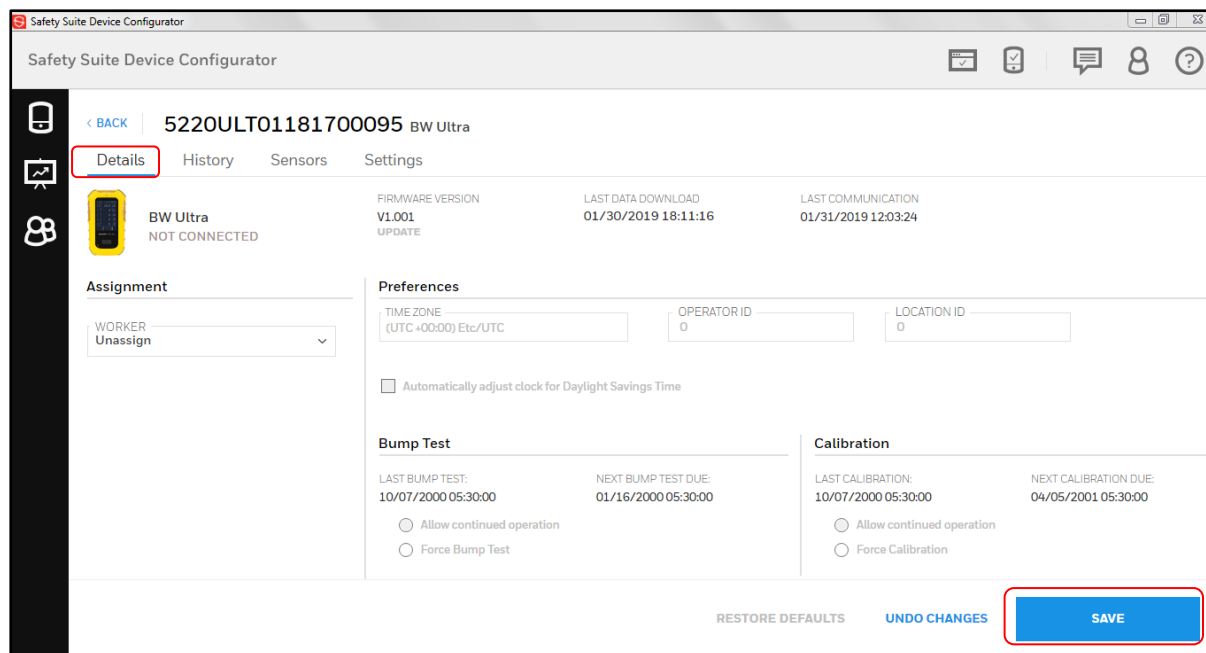

Once all the fields are filled and selected, click on **SAVE** to update the changes.

13.6.2.1 Instruments

Instruments such as gas monitors are profiled with details of bump tests, calibration, assignment, and connection with cradles and controllers. You can update the firmware, check history, sensors, and settings, and make/save changes.

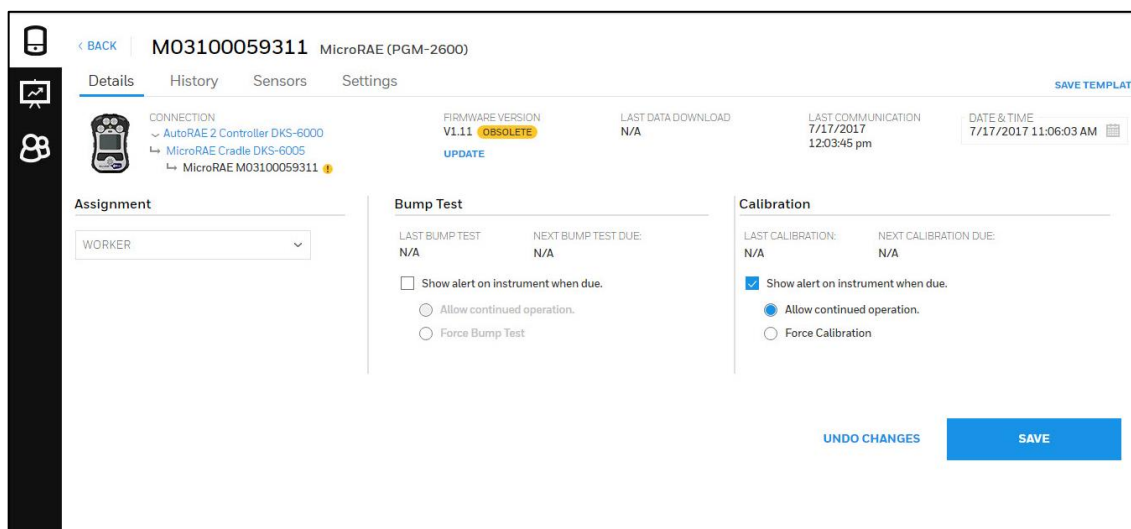

Note: If an instrument is not currently connected to the computer, under Details it says, “Not Connected-View Only”. This tells you that you cannot change settings or perform updates.

13.6.2.2 Docking Stations

Device Details for a docking station include information about gases, as well as settings. In addition, you can update the firmware version, set the Menu passcode, set date and time, and download data. You can also print calibration certificates either automatically or manually and tell the docking station to calibrate instruments if they fail a bump test.

< BACK
T021001895 AutoRAE 2 Controller (DKS-6000)

Connected REFRESH

AutoRAE 2 Controller DKS-6000

MicroRAE Cradle DKS-6005

MicroRAE M031000593...

Settings

FIRMWARE VERSION: **V1.32**

PRINT CERTIFICATES...

Automatically

Manually

PASSCODE: ********

0/4 digits remaining

Calibrate on Bump Test failure

DATE & TIME: **7/17/2017 11:08:26 AM**

LAST COMMUNICATION: **7/17/2017 12:03:45 pm**

[DOWNLOAD DATA](#)

Gas Cylinders

1 CO

GAS LOT NUMBER: ----- GAS EXPIRATION DATE: **1/1/2012**

GAS NAME	CONCENTRATION	UNIT	PURGE TIME (SEC)	SOAK TIME (SEC)
CO	50	ppm	20	0

2 CO H2S O2 Methane

GAS LOT NUMBER: ----- GAS EXPIRATION DATE: **1/1/2012**

GAS NAME	CONCENTRATION	UNIT	PURGE TIME (SEC)	SOAK TIME (SEC)
CO	50	ppm	20	0
H2S	10	ppm	20	0
O2	18	%	20	0
Methane	50	%LEL	20	0

3 Isobutylene

GAS LOT NUMBER: ----- GAS EXPIRATION DATE: **1/1/2012**

GAS NAME	CONCENTRATION	UNIT	PURGE TIME (SEC)	SOAK TIME (SEC)
Isobutylene	100	ppm	20	0

4 Isobutylene

GAS LOT NUMBER: ----- GAS EXPIRATION DATE: **1/1/2012**

GAS NAME	CONCENTRATION	UNIT	PURGE TIME (SEC)	SOAK TIME (SEC)
Isobutylene	10	ppm	20	0

5 H2S


GAS LOT NUMBER: ----- GAS EXPIRATION DATE: **1/1/2012**

GAS NAME	CONCENTRATION	UNIT	PURGE TIME (SEC)	SOAK TIME (SEC)
H2S	10	ppm	20	0

UNDO CHANGES
SAVE

13.6.2.2.1 Menu Passcode

Menu Passcode is required to access the settings menu in the physical IntelliDoX Device.

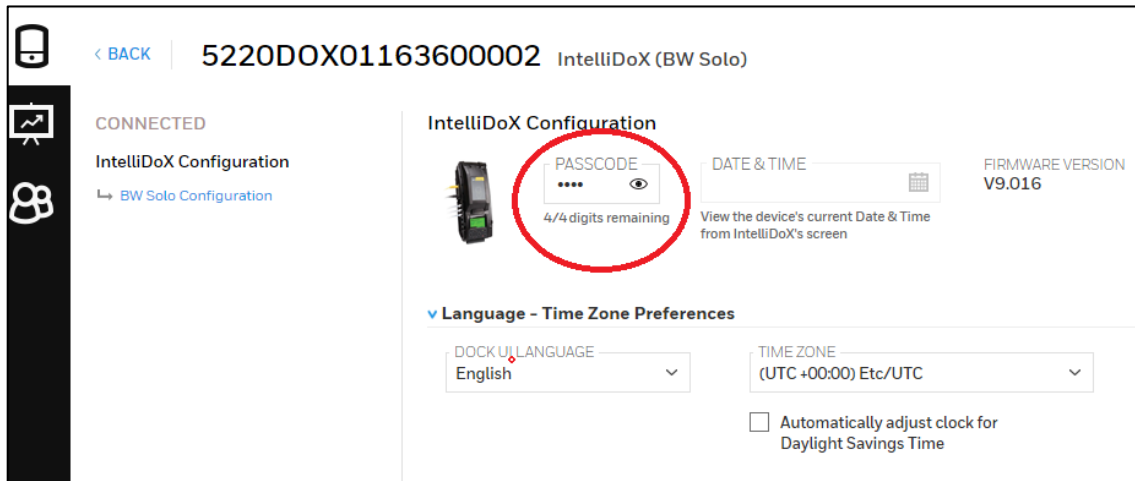


Note: User can not Set or Update/Modify Menu passcode from IntelliDoX device and can only enter this passcode to authenticate to access the IntelliDoX settings menu.

Note: The user can View or Set/Update the passcode from Device Configurator.


13.6.2.2.2 Edit Gas Cylinder Configuration

To edit a gas cylinder's configuration, click the "Edit" icon:

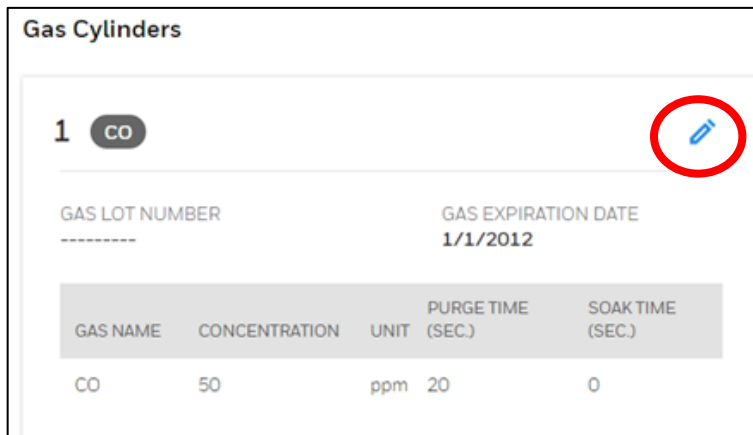



The configuration window is shown, and you can make changes to the Lot Number, Expiry (expiration date), the gas, and its attributes.

Inlet-1 Configuration

LOT NUMBER: ----- EXPIRY: 6/30/2019 

7/16 char. remaining

Gas Types and Concentrations 

GAS 1: CO CONCENTRATION: 50 ppm PURGE TIME: 20 sec. SOAK TIME: 0 sec. 

0 - 1000000 ppm 0 - 3600 sec. 0 - 3600 sec.


[UNDO CHANGES](#) [SAVE](#)

Important!


If you change any details of the configuration’s gases, make sure they match the information printed on the gas cylinder. This is especially critical for the Gas Type, Concentration (and units, such as ppm), Lot Number and Expiry date.


Add another gas (if this is a multi-gas mix) by clicking the “+” icon. Then add the details of the new gas.

Inlet-1 Configuration


LOT NUMBER: ----- EXPIRY: 1/1/2012 

7/16 char. remaining

Gas Types and Concentrations 

GAS 1: CO CONCENTRATION: 50 ppm PURGE TIME: 20 sec. SOAK TIME: 0 sec. 

0 - 1000000 ppm 0 - 3600 sec. 0 - 3600 sec.

GAS CONCENTRATION: ppm PURGE TIME: sec. SOAK TIME: sec. 

0 - 1000000 ppm 0 - 3600 sec. 0 - 3600 sec.

[UNDO CHANGES](#) [SAVE](#)


If you want to remove a gas from the list, click the “Delete” icon:



When you are done with the configuration, click “SAVE.” If you do not want to save these changes, click “Undo Changes”.

13.6.2.3 Device History

Device History provides you with data collected over time, including when calibrations and bump tests were performed, when alarm states were entered (and the type of alarm), etc. It also tells when sessions started and ended.

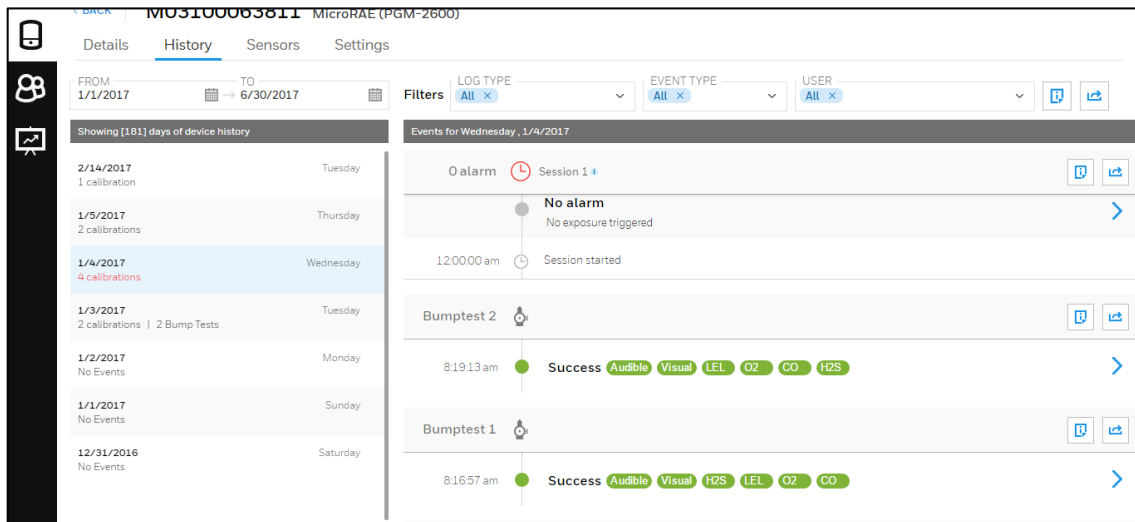


13.6.2.3.1 Filters

The data can be filtered by date range, as well as log type, event type, and user.


Date

Set your date range and click “Done.” Note: The maximum date range is one month.

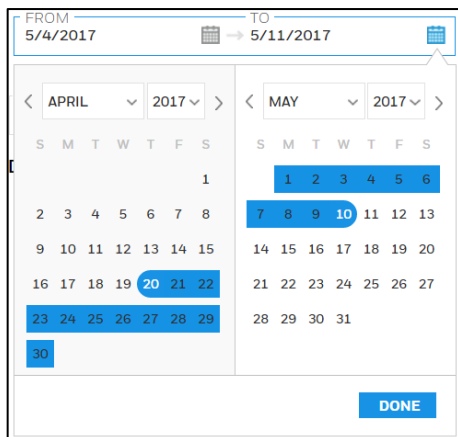

Log Type

You can choose from the available log types, including Alarm Records, Calibration, and Bump Test.

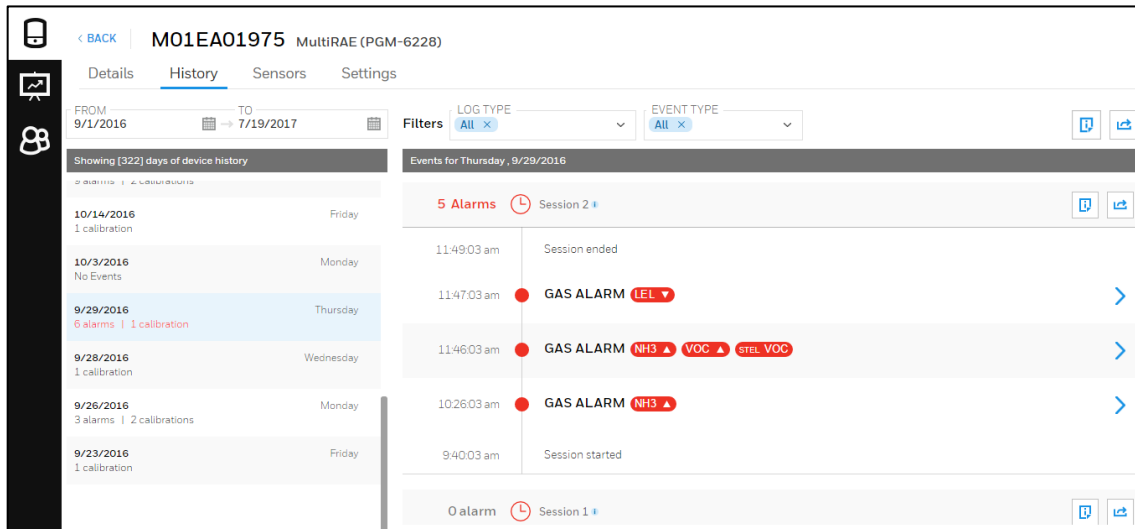

Event Type

Filter according to the type of event that is of interest.

Users

Filter according to the names of users.

Summaries

There are two ways to view summaries of a device's history.



Summary for The Day opens a window with all the day's session information, organized by session.



Export Day Info opens a window that lets you choose data elements and summary information and then export it. You can print it or save it as a CSV file for opening in a spreadsheet program such as Microsoft Excel.

Log

To view a log of a device, click the arrow icon at the right of the column:



This opens the Log window for viewing.

TIMESTAMP	CO	PPM	H2S	PPM	O2	%	LEL	%LEL
5/8/2017 9:25:14 am	0			0		20.9	0	0
5/8/2017 9:26:14 am	0			0		20.9	0	0
5/8/2017 9:27:14 am	0			0		20.9	0	0
5/8/2017 9:28:14 am	0			0		20.9	0	0
5/8/2017 9:29:14 am	0			0		20.9	0	0
5/8/2017 9:30:14 am	0			0		20.9	0	0
5/8/2017 9:31:14 am	0			0		20.9	0	0
5/8/2017 9:32:14 am	0			0		20.9	0	0

You can also view information about the session and calibration details:

SESSION SUMMARY			
ASSIGNED TO	START TIME	DURATION	RECORDS
	5/8/2017 9:25:14 am	14h 16m 0s	856
INTERVAL	END TIME		
60/sec	5/8/2017 11:41:14 pm		
SITE ID	USER ID		
SITE0000	USER0000		
CALIBRATION DETAILS			
LEL:			
LAST CALIBRATED DATE	MEASUREMENT GAS	CORRECTION FACTOR	SPAN POINT 1
4/20/2017	Methane	1	50
SPAN POINT 2			

Export

opens a window that lets you choose data elements and summary information and then export it. You can print it or save it as a CSV file for opening in a spreadsheet program such as Microsoft Excel.

Session 2 PGM-2600 MicroRAE

Log Info Export

CHOOSE DATA ELEMENTS

Timestamp Worker GPS Location

Sensor Reading

Alarm Type for Each Sensor

Alarm type for Each Record

Unit of Measure

CHOOSE SUMMARY INFORMATION

Session information Operation information Calibration information

Sensor information Assignment information

CANCEL EXPORT

13.6.2.4 Sensors

Select “Sensors” to view and edit attributes of sensors installed in a device.

< BACK M03100059311 MicroRAE (PGM-2600)

Details History **Sensors** Settings MULTICALIBRATION MANAGE GAS LIST SAVE TEMPLATE

LEL - LEL

Alarm Setpoints	Calibration	Bump Test
LOW ALARM 15%LEL	Last: N/A Next: 4/20/2017 INTERVAL 0days	Last: N/A Next: 4/20/2017 INTERVAL 0days
HIGH ALARM 25 %LEL	CALIBRATED TO CH4	
OVER RANGE 100%LEL	MEASURING CH4	
	SPAN LEVEL 50%LEL	

O2 - Oxygen

Alarm Setpoints	Calibration	Bump Test
LOW LOW ALARM 17.0% Vol	Last: N/A Next: 4/20/2017 INTERVAL 0days	Last: N/A Next: 4/20/2017 INTERVAL 0days
LOW ALARM 19.5% Vol	SPAN LEVEL 18.0% Vol	
HIGH ALARM 23.5 % Vol		
OVER RANGE 30.0% Vol		

CO - Carbon Monoxide

Alarm Setpoints	Calibration	Bump Test
LOW ALARM 35 ppm	Last: N/A Next: 4/20/2017 INTERVAL 0days	Last: N/A Next: 4/20/2017 INTERVAL 0days
HIGH ALARM 200 ppm	SPAN LEVEL 50ppm	
OVER RANGE 1000 ppm		
STEL ALARM 100 ppm		
TWA ALARM 35 ppm		

H2S - Hydrogen Sulfide

Alarm Setpoints	Calibration	Bump Test
LOW ALARM 10.0 ppm	Last: N/A Next: 4/20/2017 INTERVAL 0days	Last: N/A Next: 4/20/2017 INTERVAL 0days
HIGH ALARM 20.0 ppm	SPAN LEVEL 10.0 ppm	

13.6.2.5 Settings

View and manage settings in a device. You can save these as a file or as a template.


The screenshot shows the settings interface for a MicroRAE (PGM-2600) device. The device ID is M03100059311. The settings are organized into several sections:

- GAS ALARMS:** ALARM TYPE is set to 'Auto-Reset' and ALARM INDICATORS is set to 'All Disabled'.
- MAN-DOWN ALARMS:** ALARM SENSITIVITY is 'High', MAN-DOWN CUSTOM SENSITIVITY is '64', and PRE-ALARM AFTER is '30' seconds. There is also a 'FULL ALARM AFTER' field set to '30' seconds and a 'Man-Down If Motionless' checkbox.
- DATALOGGING:** LOG ONCE EVERY is '60' seconds. LOGGED MEASUREMENTS includes 'Minimum', 'Average', 'Maximum', and 'Real Time'. AVERAGE TYPE is 'Moving average'. LOG MAP includes 'LEL', 'O2', 'CO', and 'H2S'. LOG START TYPE is 'Auto' and LOG MEMORY FULL ACTION is 'Wraparound'.
- INSTRUMENTS OPERATION:** 'Comfort Beep' and 'Startup Speed' are both checked.
- System Options:** 'Auto Zero' is unchecked.
- Gas Setting:** 'GLANCE OPTION ENABLE' is 'Enabled' and 'GLANCE ITEM' includes 'Configurate...' and 'Wireless typ...'.
- INSTRUMENT USER PREFERENCES:** SITE ID is 'SITE0000', USER ID is 'USER0000', and PASSCODE is '****'. USER MODE is 'Basic', BACK LIGHT OPTION is 'Manual', and BACK LIGHT TRIGGER is '2200'. LCD CONTRAST is '50%' and LED Status is checked. BLINK INTERVAL LED is '3' seconds.

At the bottom right, there are 'UNDO CHANGES' and 'SAVE' buttons.

Jump to


The section labeled “Jump to” provides rapid navigation, especially useful when many details are included in Settings and would otherwise require scrolling up and down. Click a heading, and that section of Settings becomes the focus.

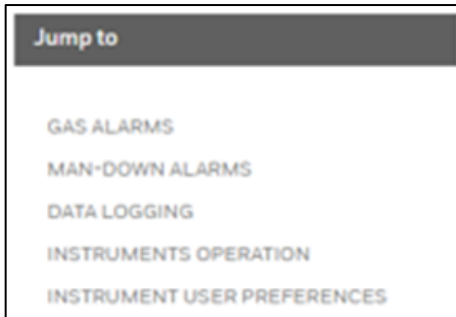

13.6.3 Custom fields in Device Configurator

User can add new Custom fields (User defined fields) to capture additional information about devices.

To add new Custom fields, Open the Devices tab and click on **Custom fields** then you can see the **ADD FIELD** option to add the new Custom field.

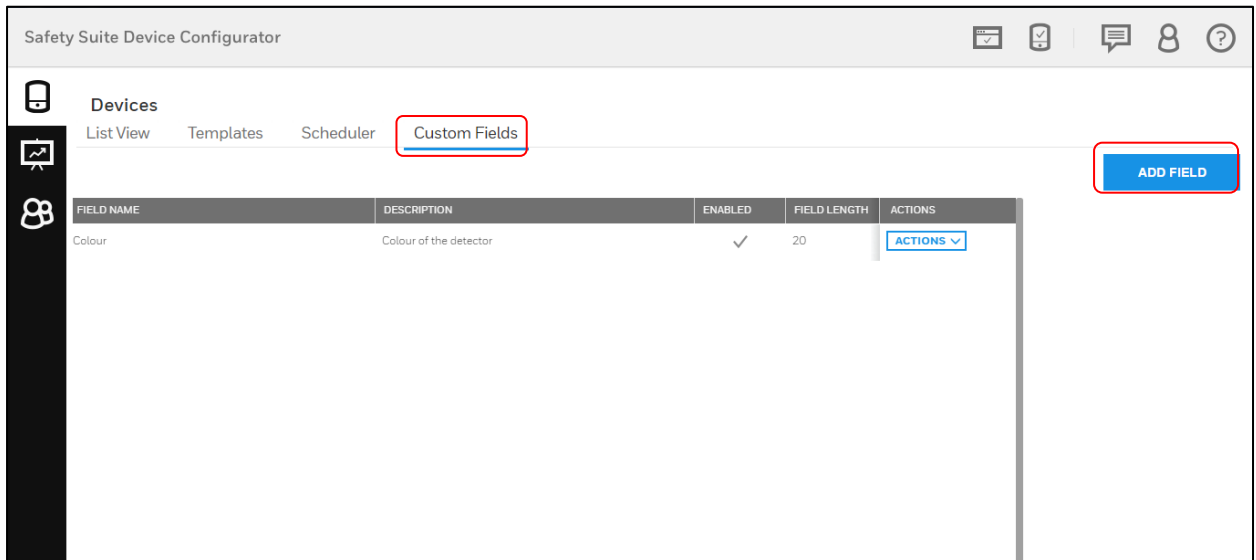


After clicking on **ADD FIELD**, a popup screen will open. User can fill the required details as follows.

Field Name: User can type in the field label (e.g. “Device Location” or “Device color”)

Field Description: User can give a brief Description about the field. This information is not displayed in the device detail view.

Max Field Length: The maximum length of data in characters that this field can take. This can be set from 1 to 255 characters.

Enabled: This option enables the newly added custom field. Enabling a field will make it available for all devices and users can view the data for these fields in the List View. A maximum of four custom field can be activated in the application. You may however change a field to/from Enabled at any time.

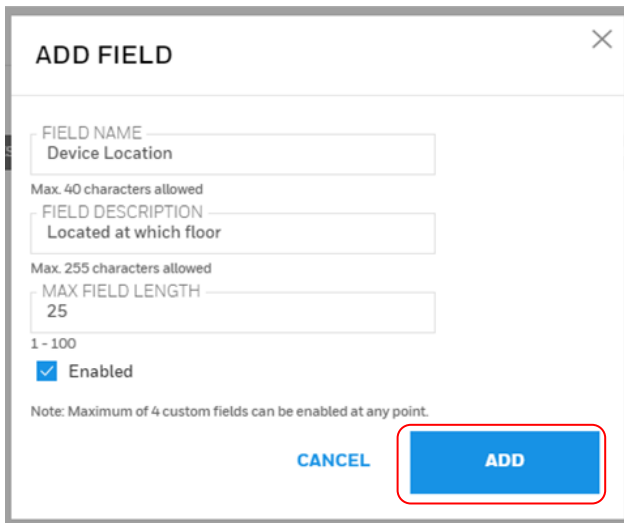

ADD FIELD

FIELD NAME
Device Location

Max. 40 characters allowed

FIELD DESCRIPTION
Located at which floor

Max. 255 characters allowed

MAX FIELD LENGTH
25

1 - 100


Enabled

Note: Maximum of 4 custom fields can be enabled at any point.

CANCEL ADD

Once all the details are filled, then click on **Add** to save the Custom field.

After successfully adding the custom field, click on the **columns** option as shown below. Please note that the device list needs to be refreshed for the custom fields to be displayed.

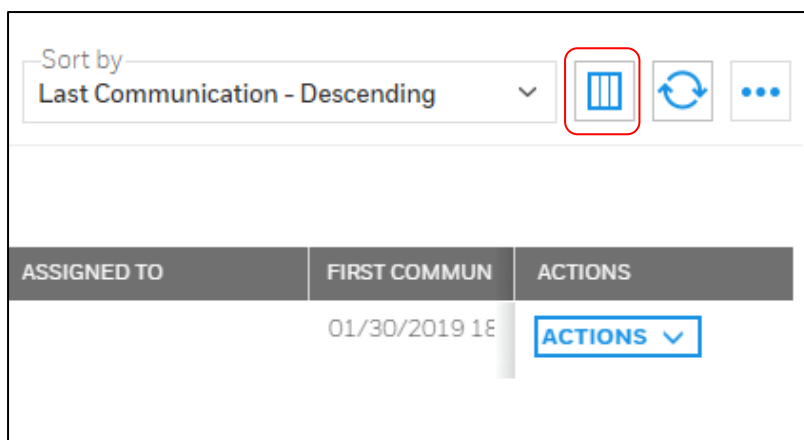


Sort by
Last Communication - Descending


Columns Refresh More

ASSIGNED TO	FIRST COMMUN	ACTIONS
	01/30/2019 1E	ACTIONS


A Pop up of Columns is displayed, enable the check box of the custom field that you have added newly, then click on DONE.

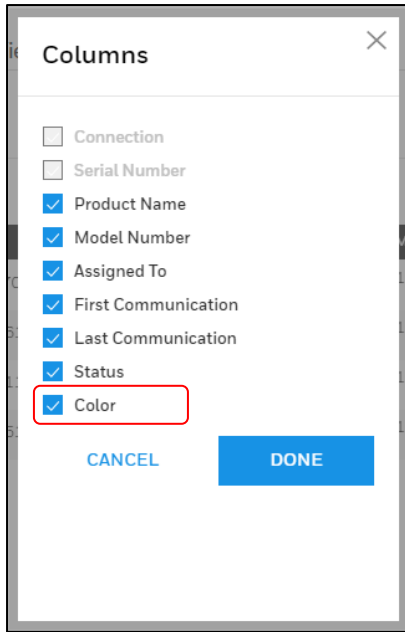


To view the newly added custom field scroll the grid column towards right-end side.

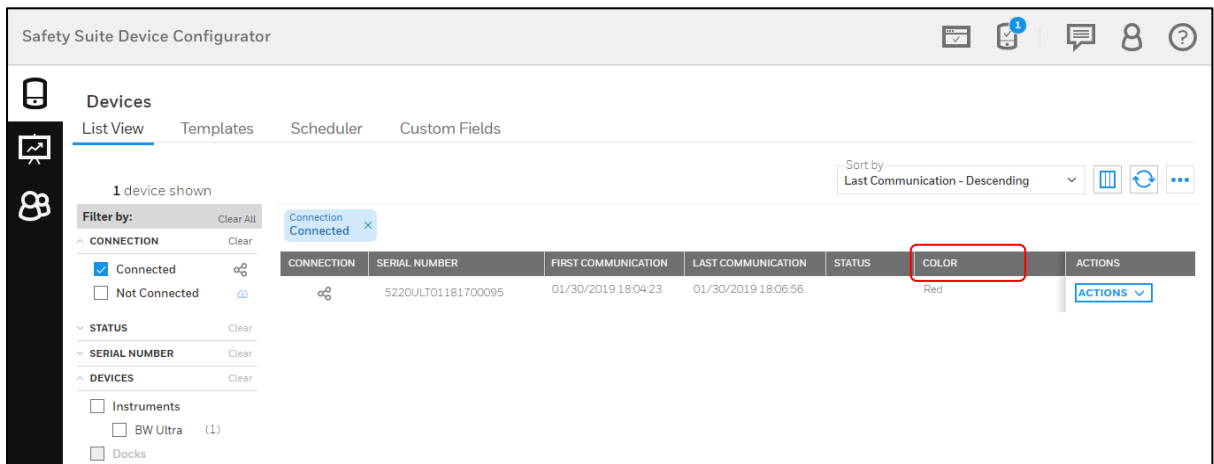


To view or edit the custom field values for a specific instrument, click on the “Action” dropdown list and select “Device Details”.

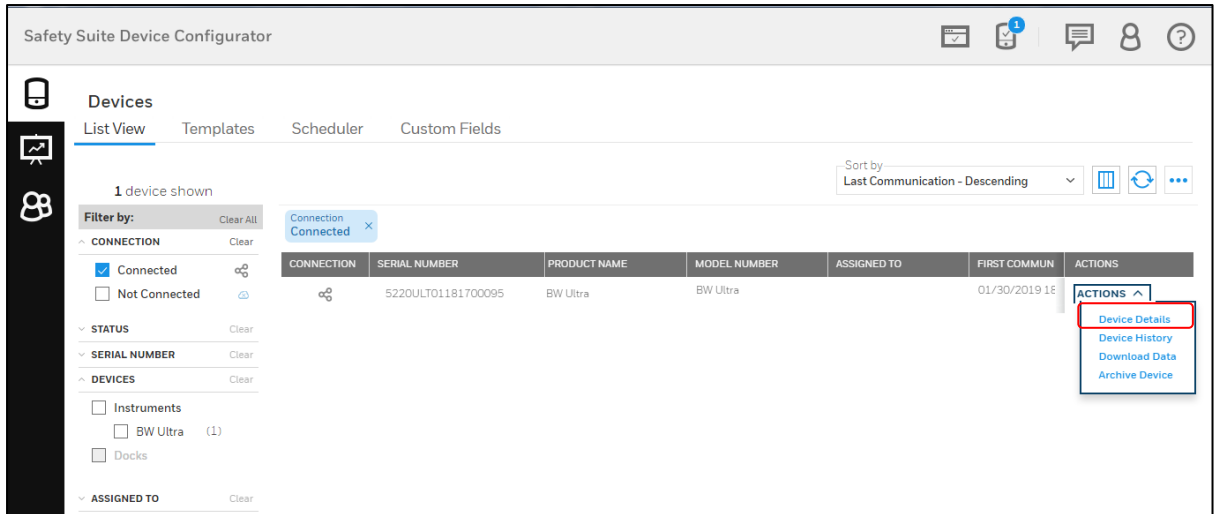

After clicking on “Device Details” below screen will open and enter the custom field value and click on SAVE.

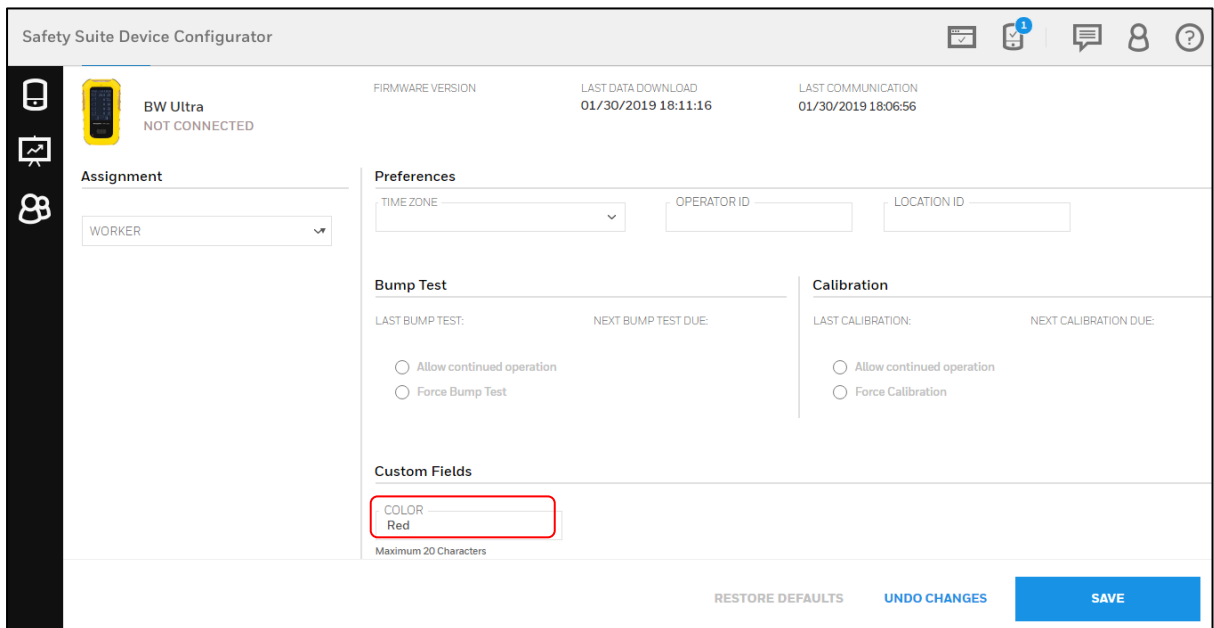

Now open the **Device** view and click on **List view**, the below screen you can see the value for custom field that you updated.

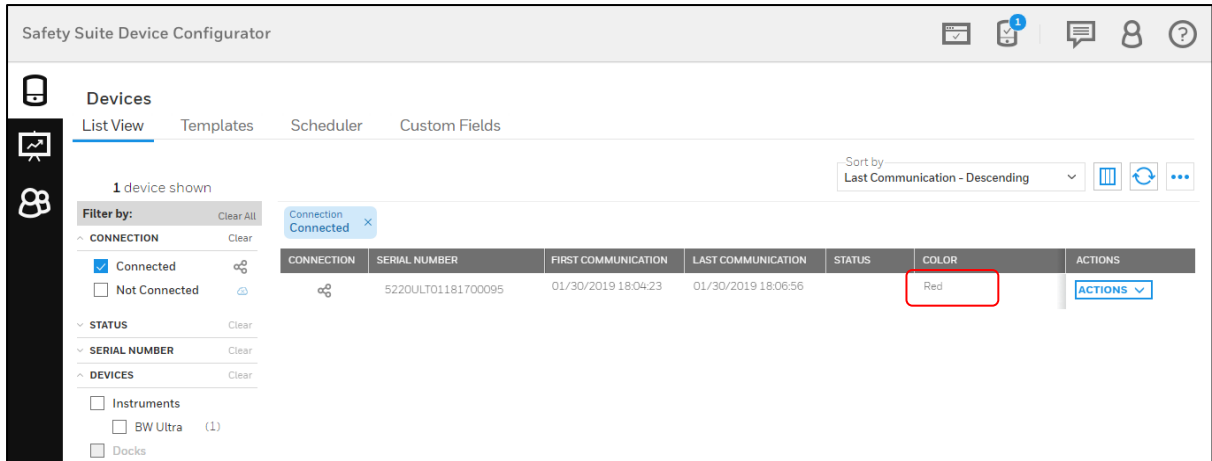


13.6.4 Download Data

Click this to download data from a device into SAFETY SUITE DEVICE CONFIGURATOR.


Note: The download time depends on the amount of data stored in the device.

13.6.4.1 Data download from Multiple Intellidox

User can initiate data download from multiple devices at the same time. Connect the devices and select 'Download Data' from one or more Intellidox devices.

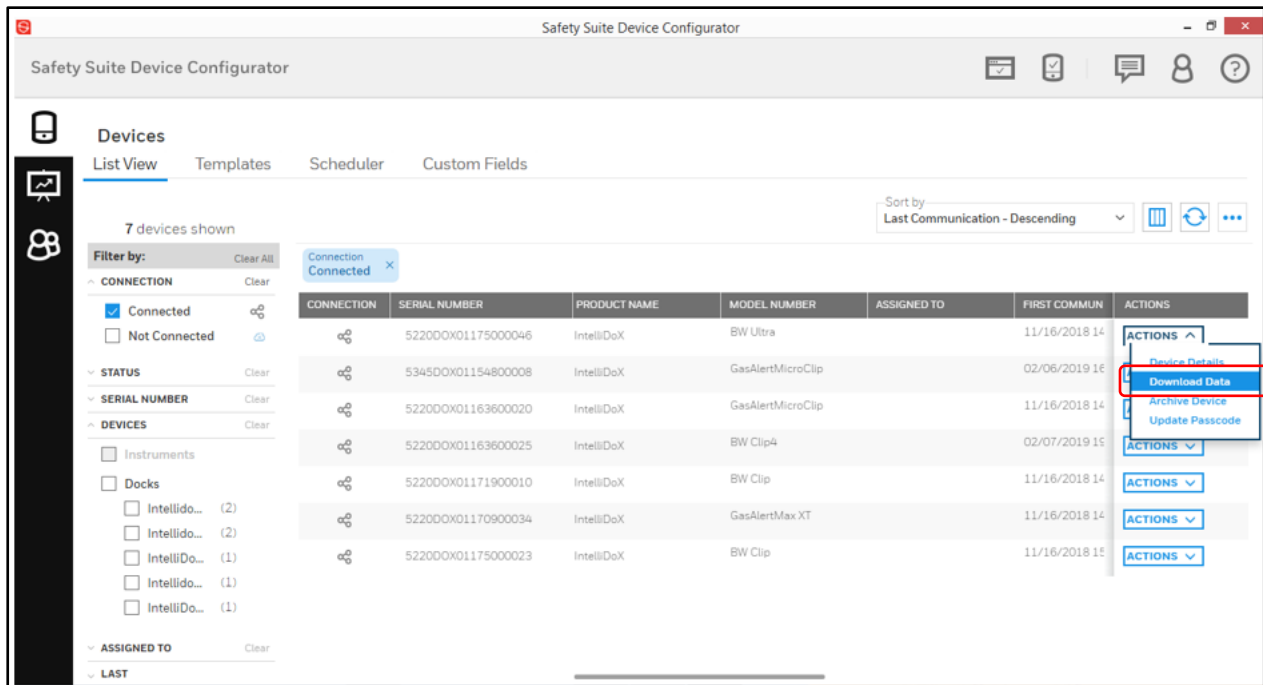


All downloads will be queued and processed. The status is visible in the queue manager and user can cancel the downloads which are in queue or in progress.

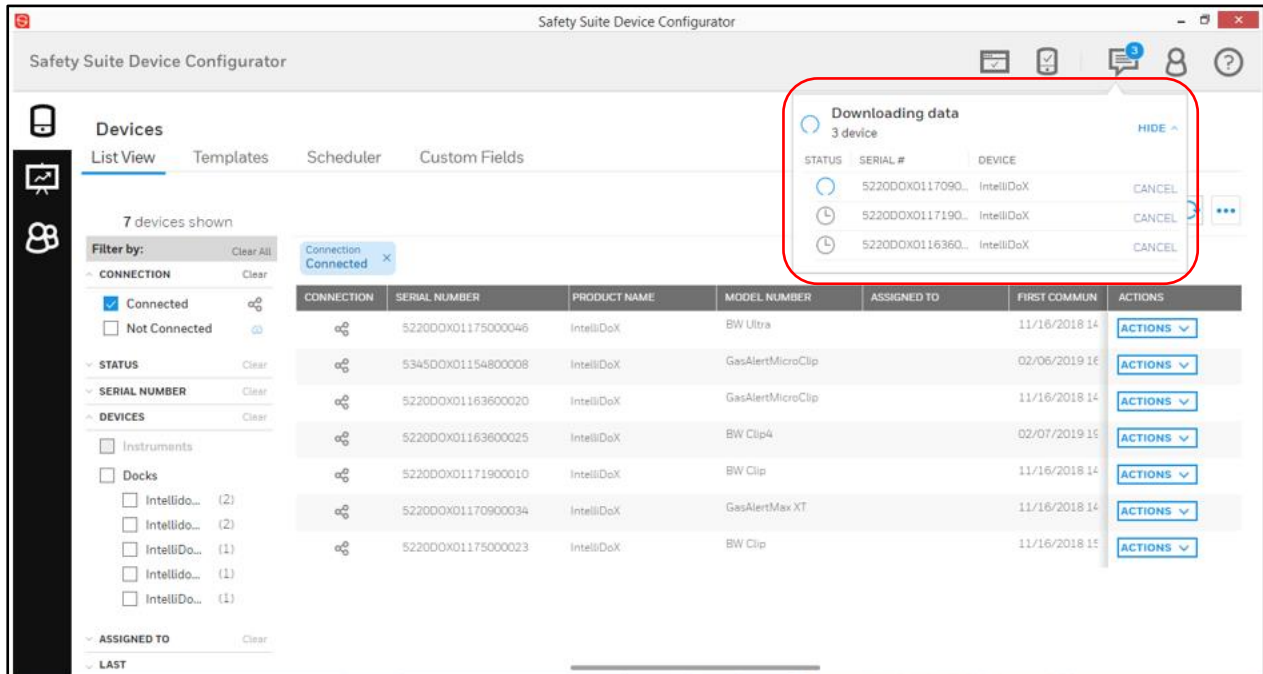

13.6.4.2 Scheduled data import

User can Schedule automatic import/download data from docking stations. Below are the steps to be followed to set up the scheduled data import.


Step 1- Click on **Devices** icon and select the **Scheduler** option to set the time.

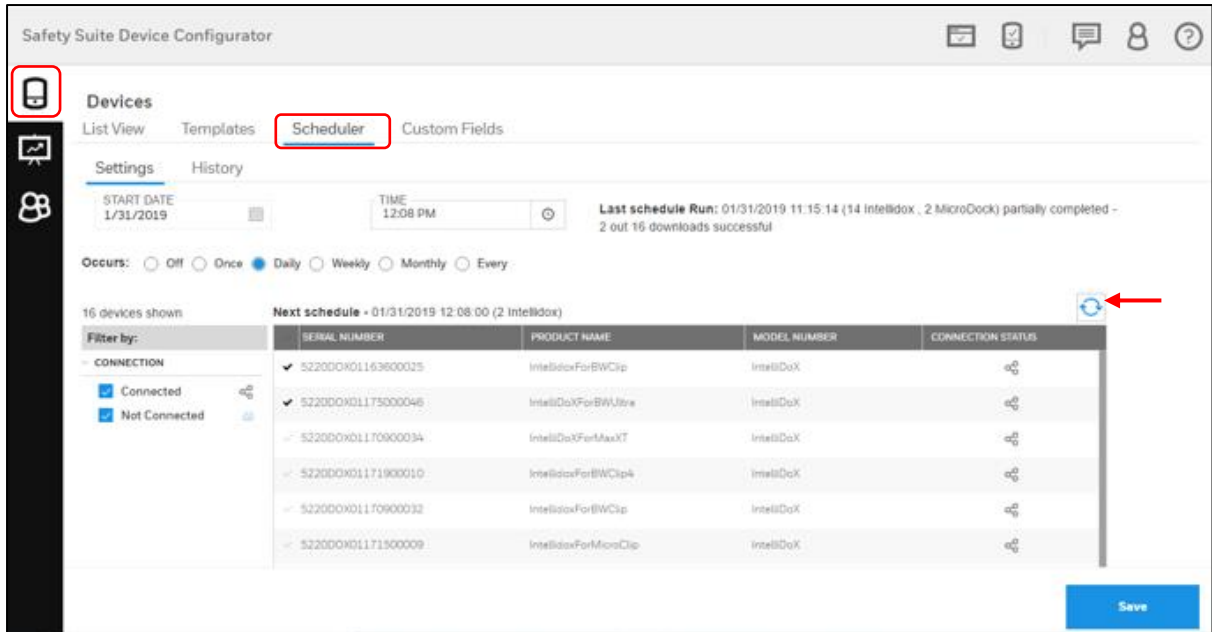

Note-Before making your selection, please refresh the docking station connectivity status by clicking the refresh button.

Step 2- Set the START DATE and TIME by clicking on the **Settings** tab and select the OCCURS options when user want to run the download.

Note-Make sure Schedule Start Date Time should be greater than current date time.

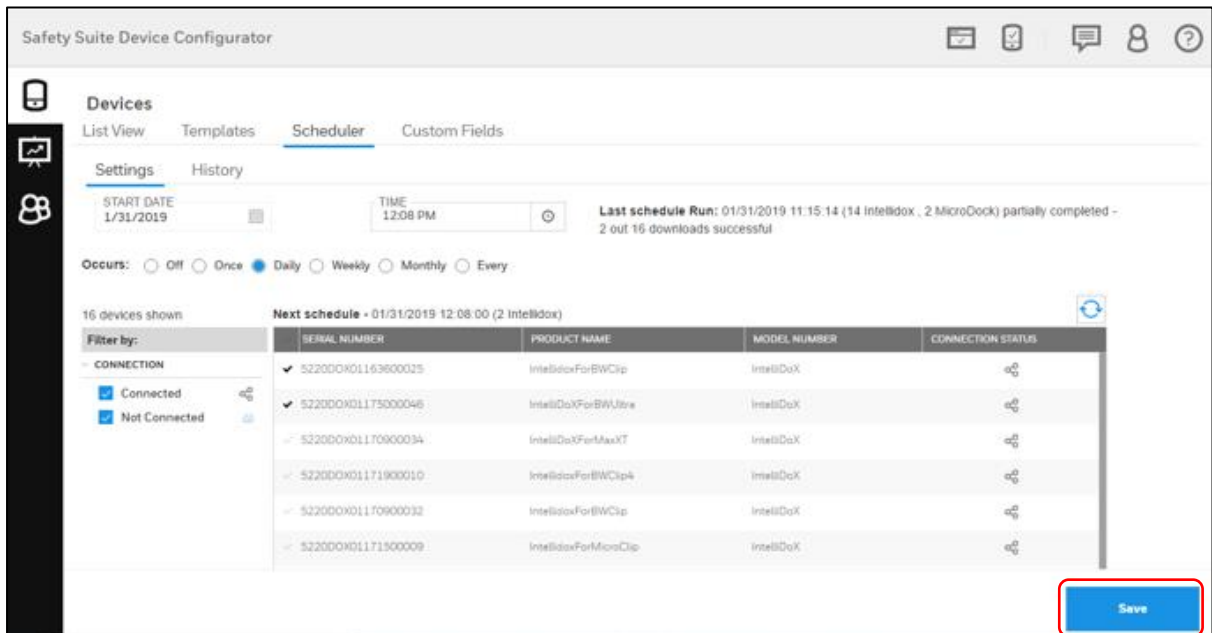

Step 3- After you select the scheduled date and time, click on **SAVE** button.

User can also see the Last schedule run details and Next schedule details in the below screen.

The screenshot shows the 'Scheduler' tab in the 'Safety Suite Device Configurator'. The 'Settings' section includes a 'START DATE' of 1/31/2019 and a 'TIME' of 12:08 PM. The 'Occurs' section is set to 'Daily'. A 'Last schedule Run' summary indicates a run on 01/31/2019 at 11:15:14, with 14 Intelidox and 2 MicroDock devices partially completed, and 2 out of 16 downloads successful. A table below shows the 'Next schedule' for 01/31/2019 at 12:08:00, listing 2 Intelidox devices. A 'Save' button is highlighted in the bottom right corner.


SERIAL NUMBER	PRODUCT NAME	MODEL NUMBER	CONNECTION STATUS
5220DOX01163600025	IntelidoxForBWCip	Intelidox	Connected
5220DOX01175000046	IntelidoxForBWUltra	Intelidox	Connected
5220DOX01170900034	IntelidoxForMaxXT	Intelidox	Not Connected
5220DOX01171900010	IntelidoxForBWCip4	Intelidox	Not Connected
5220DOX01170900032	IntelidoxForBWCip	Intelidox	Not Connected
5220DOX01171900009	IntelidoxForMicroClip	Intelidox	Not Connected

Step 4- When scheduled time approaches, it will show the scheduled progress details and if user want to cancel the scheduled progress, click on cancel button.


The screenshot shows the 'Scheduler' tab with the 'Occurs' section set to 'Daily'. A 'Current Schedule: In Progress - (2 Intelidox)' notification is displayed with a 'Cancel' button. The 'Next schedule' is now for 02/01/2019 at 12:08:00, listing 2 Intelidox devices. The table below shows the next scheduled devices.

SERIAL NUMBER	PRODUCT NAME	MODEL NUMBER	CONNECTION STATUS
5220DOX01163600025	IntelidoxForBWCip	Intelidox	Connected
5220DOX01175000046	IntelidoxForBWUltra	Intelidox	Connected
5220DOX01170900034	IntelidoxForMaxXT	Intelidox	Not Connected
5220DOX01171900010	IntelidoxForBWCip4	Intelidox	Not Connected
5220DOX01170900032	IntelidoxForBWCip	Intelidox	Not Connected
5220DOX01171900009	IntelidoxForMicroClip	Intelidox	Not Connected
5220DOX01175000023	IntelidoxForBWCip	Intelidox	Not Connected
5220DOX01171400014	IntelidoxForBWUltra	Intelidox	Not Connected

Step 5- After completing the scheduled run process, click on **History** and check the scheduled run status. User can also check the older data details by changing the Date Range option.

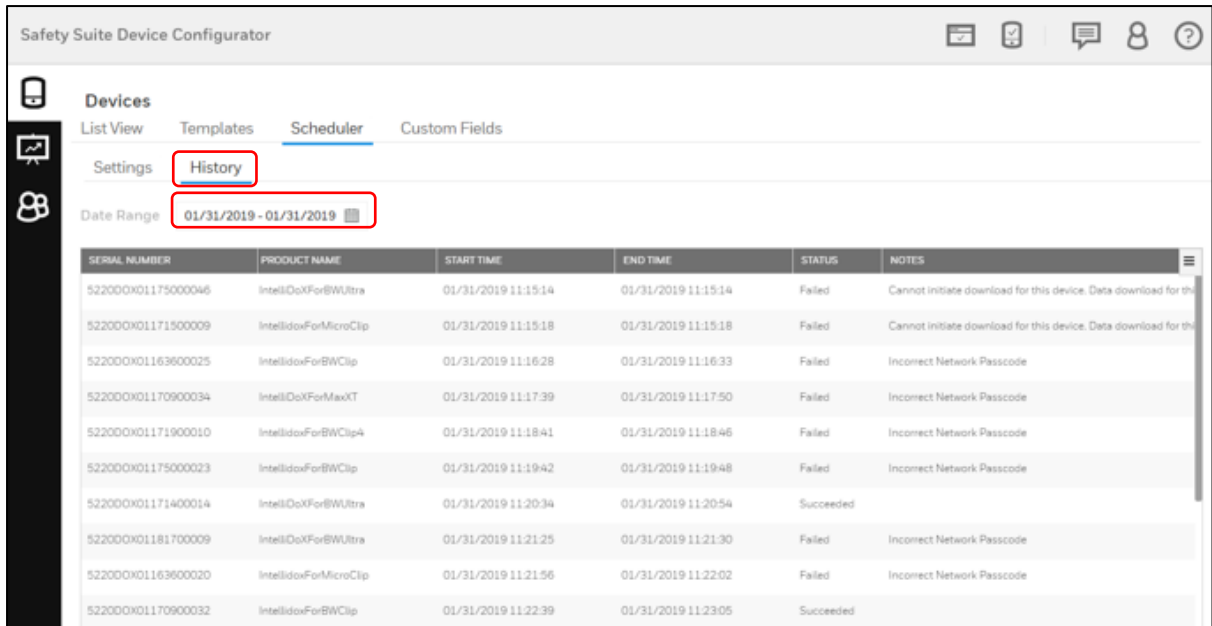


Step 6- If user want to export the data, click on below show n red marked box and export the data to CSV file.

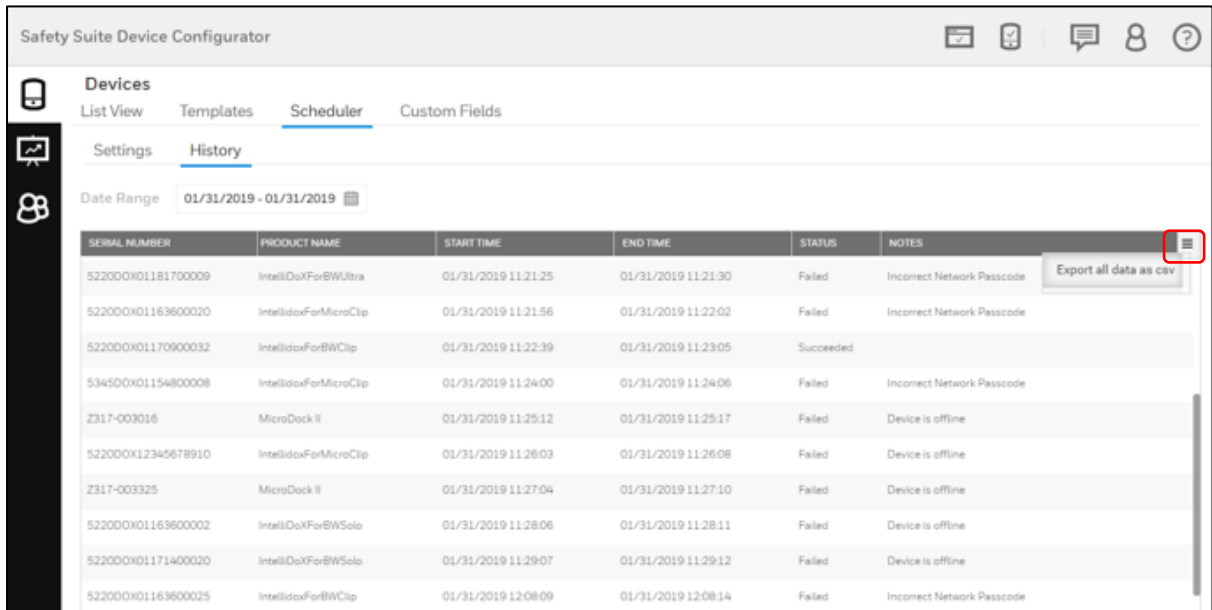

The scheduler does not require the user to remain logged in during the data download. If the system is re-started, while the schedule is in progress, the remaining downloads will appear in the Queue manager and will resume download to the extent possible. Please note if you login to the application when the scheduled download is in progress, the in-progress downloads will appear in the queue manager.


13.6.5 Archive Device

Click this choice to de-assign a device from a user and make it invisible to the default device list.

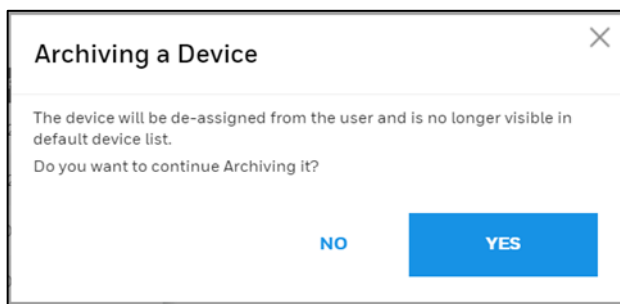

13.6.6 Network Passcode

The Network Passcode is required to access IntelliDoX to perform any ACTION, the passcode is defined to access and operate or change setting in IntelliDoX over the network.

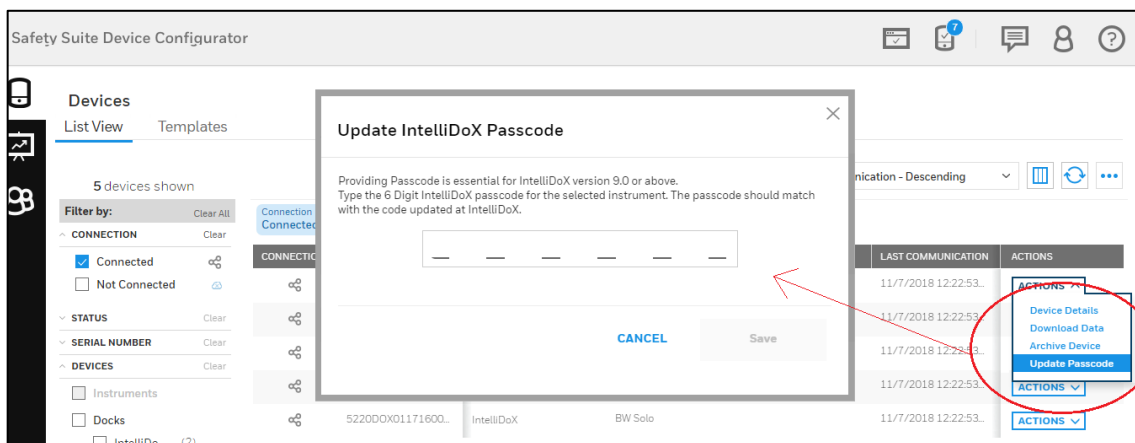

Network Passcode is applicable/available on IntelliDoX device having firmw are 9.0 and above only.



Note: The user can not Set or Update/Modify passcode from Device Configurator and can only enter this passcode to authenticate and access the IntelliDoX to perform any ACTION.


Note: The user can View or Set/Update the Network passcode in IntelliDoX Device.

13.7 Save Template

You can save the device's settings as a template. Click "Save Template."

13.7.1 Templates


You view or edit templates containing settings from instruments. Edited templates can be saved and recalled for one instrument or many.

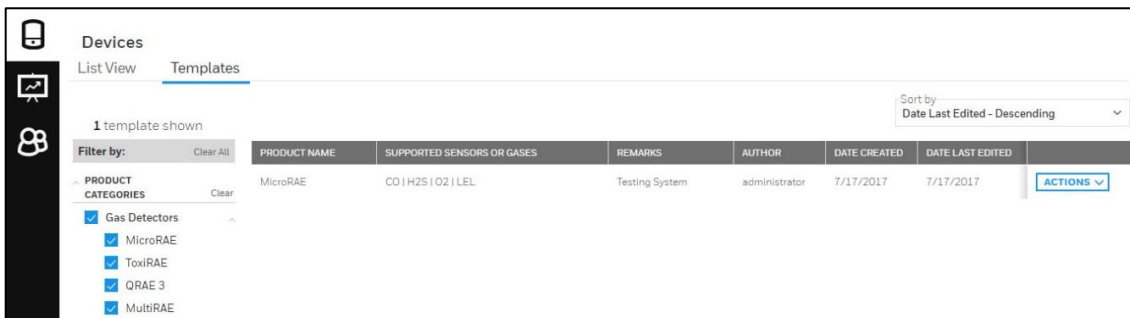

[< BACK](#) | MicroRAE (PGM-2600) Template

Settings | Sensor

Template Description:



Model: MicroRAE - CO | H2S | O2 | LEL
 Author: administrator
 Date Created: 4/18/2017
 Last Edit: 4/18/2017

Bump Test

Show alert on instrument when due.

Allow continued operation.
 Force bump test.

Calibration

Show alert on instrument when due.

Allow continued operation.
 Force calibration.

GAS ALARMS

ALARM TYPE: Auto-Reset | ALARM INDICATORS: Light only

MAN-DOWN ALARMS

ALARM SENSITIVITY: High | MAN-DOWN CUSTOM SENSITIVITY: 64 | PRE-ALARM AFTER: 30 sec
30-90 sec.

FULL ALARM AFTER: 30 sec | Man-Down If Motionless
30-90 sec.

DATALOGGING

LOG ONCE EVERY: 60 sec | LOGGED MEASUREMENTS: Minimum X Average X Maximum X Real Time X
1-3600 sec. Default: 60 sec.

AVERAGE TYPE: TWA | LOG MAP: LEL X O2 X CO X H2S X

LOG START TYPE: Auto | LOG MEMORY FULL ACTION: Wraparound

INSTRUMENTS OPERATION

Comfort Beep | Startup Speed

System Options

Auto Zero

Gas Setting

GLANCE OPTION ENABLE: Enabled | GLANCE ITEM: Configure... X Wireless typ... X

INSTRUMENT USER PREFERENCES


SITE ID: SITE0000 | PASSCODE: **** | USER MODE: Basic
0/8 char. remaining(ABCD1234) | 0/4 digits remaining(digits only)

BACK LIGHT OPTION: Auto | BACK LIGHT TRIGGER: 2200 | LCD CONTRAST: 50 %
1500 - 2600 | 0 - 100%

LED Status | BLINK INTERVAL LED: 3 sec
1 - 60 sec.

[UNDO CHANGES](#) [SAVE](#)


When you have finished editing a template, you can save it or undo the changes. Before you make any edits, the choices labeled “UNDO CHANGES” and “SAVE” are gray and cannot be used. Once changes have been made, the buttons are activated and can be used.



changes to...




When you save a template, a “Save Template?” dialog is displayed. You can add remarks, and select whether you want to see the new template after saving it.

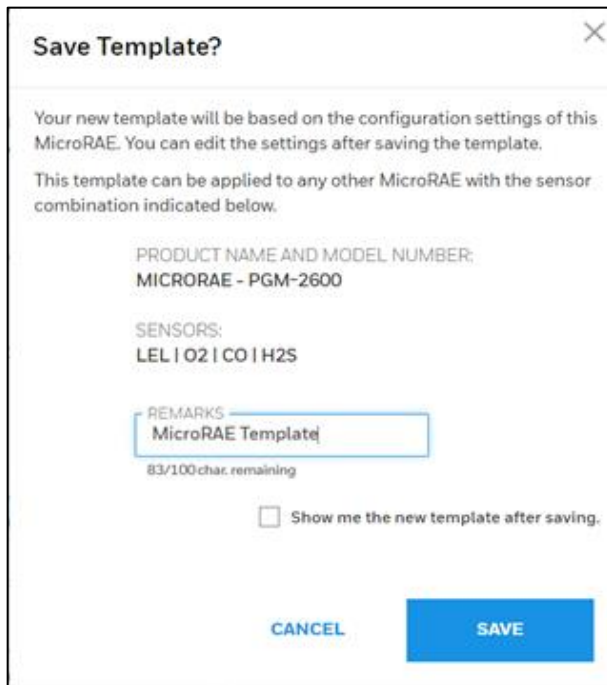



13.8 IntelliDoX USB Data Download

You can copy IntelliDoX data files to a USB storage device and physically transfer them to the computer running Safety Suite Device Configurator. Plug in a USB storage device (stick, external hard drive, etc.) into the IntelliDoX USB port, copy the data files to the USB device, and then plug the USB device into the computer running Safety Suite Device Configurator.

Select “Download IntelliDoX data” to select the location of the data folder on the USB device to begin the transfer.

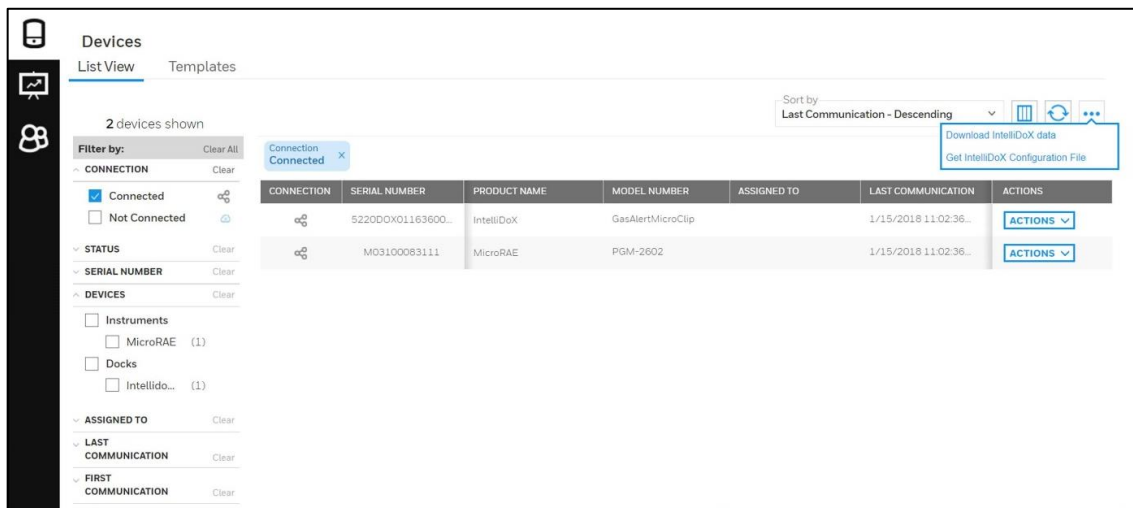

A message is shown to indicate that the data download has started:

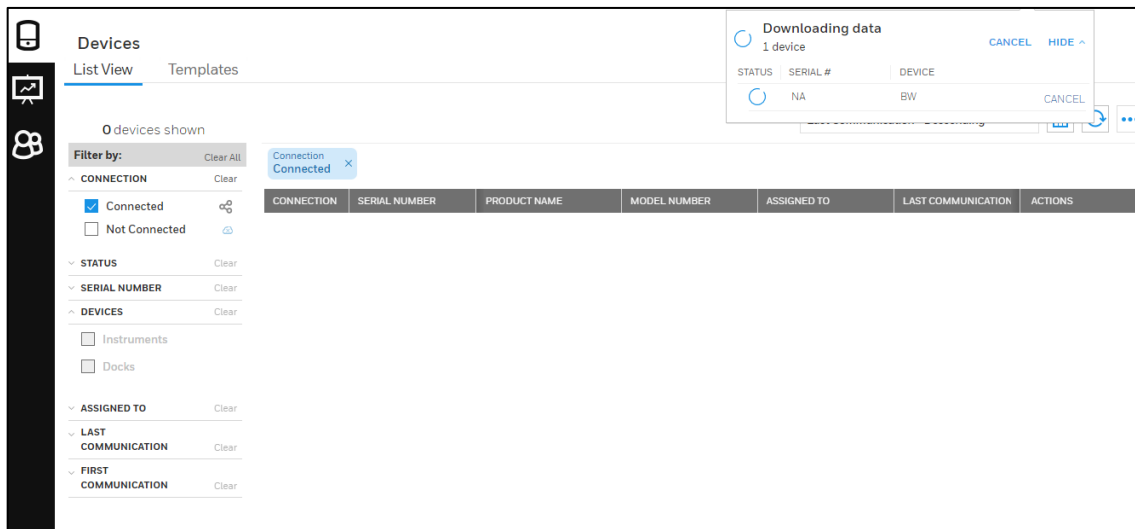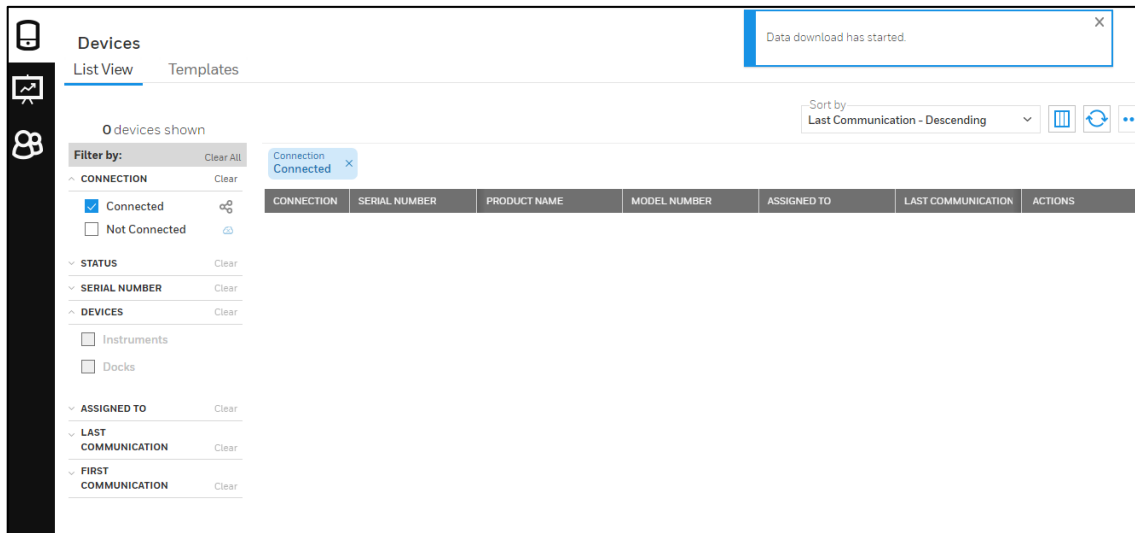


This imports the data log, test log, and event log files into Safety Suite Device Configurator as if download were initiated through IntelliDoX.

13.9 IntelliDoX USB Configuration Management


Safety Suite Device Configurator provides the ability to open and read the configuration file copied from IntelliDoX using a USB memory device to transfer and modify the parameters, save the file back to the USB device, and then transfer it through USB port back to IntelliDoX, to apply the modifications.

Copy the IntelliDoX configuration file from the IntelliDoX using a USB memory device. Select the option "Get IntelliDoX Configuration File" to point to the IntelliDoX file (which has an extension of .cof). Once the valid file is provided,

Safety Suite Device Configurator prompts you to select the type of instrument that is appropriate to your configuration.

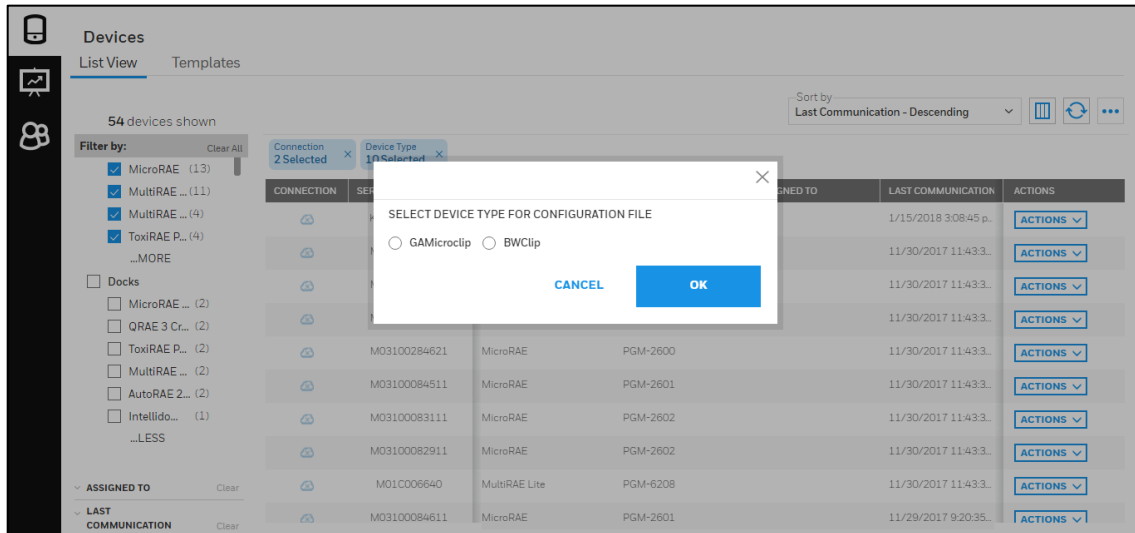


This screen shows a selection of a GAMicroClip:

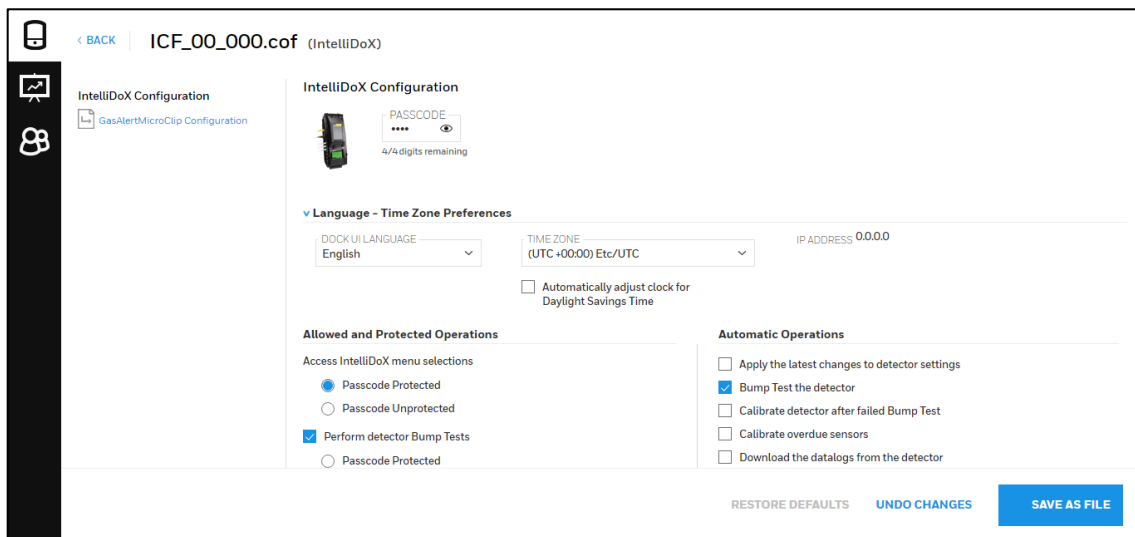

You can now customize the parameters (similar to modifying them when connected directly to IntelliDoX). Then select the option "SAVE AS FILE" to copy the modification and apply the changes to desired IntelliDoX.



13.10 User List

The User List shows all users registered with **Safety Suite Device Configurator**, regardless of whether they are Active Users, Locked Users, or Deactivated Users. The roster can be filtered in a variety of ways for organization or searching.

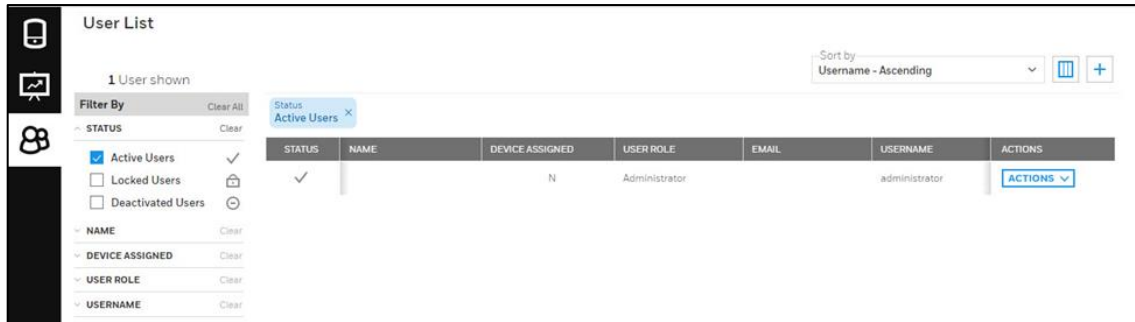

13.10.1 Sort by

Use this pulldown menu to sort your templates for quicker searching, greatest current relevance, or other ways that suit your workflow.

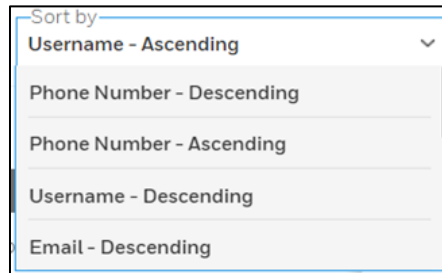

- Username – Ascending**
- Phone Number – Descending**
- Phone Number – Ascending**
- Username – Descending**
- Email – Descending**
- Email – Ascending**
- User Role – Descending**
- User Role – Ascending**
- Device Assigned – Descending**
- Device Assigned – Ascending**
- Name – Descending**
- Name – Ascending**


13.10.2 Columns

Click “Columns” to open a menu where you can select columns you want to appear on the screen:



Columns

Click a box to show a check mark, which indicates that you have selected this column to be shown. Boxes/names in light gray indicate that their visibility cannot be changed. When you have finished with your selections, click “Done” to save your choices or “Cancel” to keep your current choices.

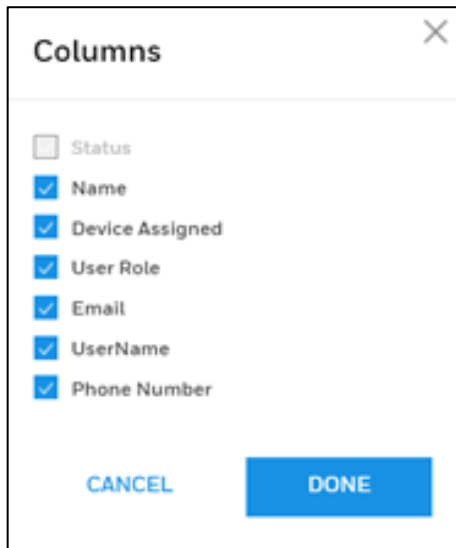

13.10.3 Actions

Depending on the user’s role, actions can include User Details, Activate User (or Deactivate User), or Delete User.




User Details is the default view. It shows each user according to filter settings, as well as all details defined in the Columns settings.

Activate User/Deactivate User gives control over who can be considered an active user. An active user is someone who has access to a device, whereas a deactivated user is not granted access (whether temporarily or permanently). A deactivated user can be re-activated.

Delete User is where you remove a user from the roster, such as when an employee leaves a company, is transferred elsewhere, etc. **Note:** If a user is deleted, their profile is deleted. This is permanent, so you cannot restore a deleted user to an active user status.

13.10.4 Add A User

Click the “+” button to open a page where you fill in information and create the profile for a new user.

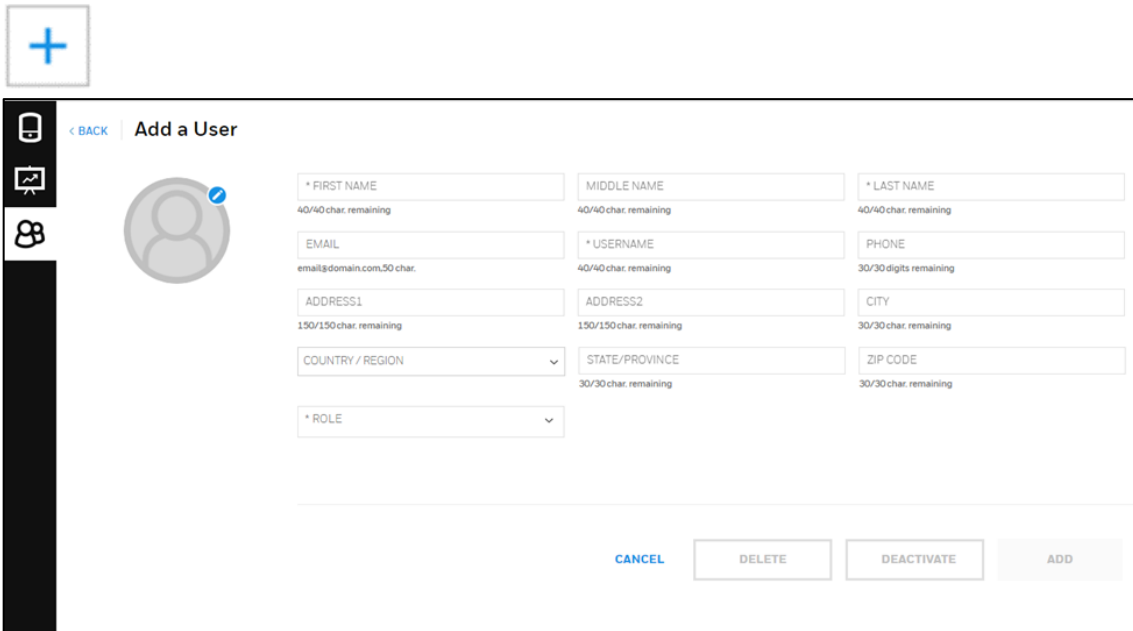


The screenshot shows a mobile application interface for adding a new user. At the top left, there is a blue plus sign button. Below it is a navigation bar with a back arrow and the text "Add a User". To the left of the form is a vertical sidebar with icons for a mobile phone, a document, and a group of people. The main form area contains several input fields: * FIRST NAME (40/40 char. remaining), MIDDLE NAME (40/40 char. remaining), * LAST NAME (40/40 char. remaining), EMAIL (email@domain.com, 50 char.), * USERNAME (40/40 char. remaining), PHONE (30/30 digits remaining), ADDRESS1 (150/150 char. remaining), ADDRESS2 (150/150 char. remaining), CITY (30/30 char. remaining), COUNTRY / REGION (dropdown), STATE / PROVINCE (30/30 char. remaining), ZIP CODE (30/30 char. remaining), and * ROLE (dropdown). At the bottom right of the form, there are four buttons: CANCEL, DELETE, DEACTIVATE, and ADD. The ADD button is highlighted in blue.

You must provide a First Name, Last Name, Email address, and Username, plus you must select a role (or roles). All other information is optional. Once you have provided the necessary information and selected a role, “Add” is highlighted. Click this to add the new user to the roster. If you do not want to save it, click “Cancel.”



This image shows a close-up of the bottom buttons from the form. There are four buttons: CANCEL (blue text), DELETE (grey text), DEACTIVATE (grey text), and ADD (white text on a blue background). The ADD button is highlighted.

After you add a new user, a message is shown that tells you the new user must provide an activation code during their first login.

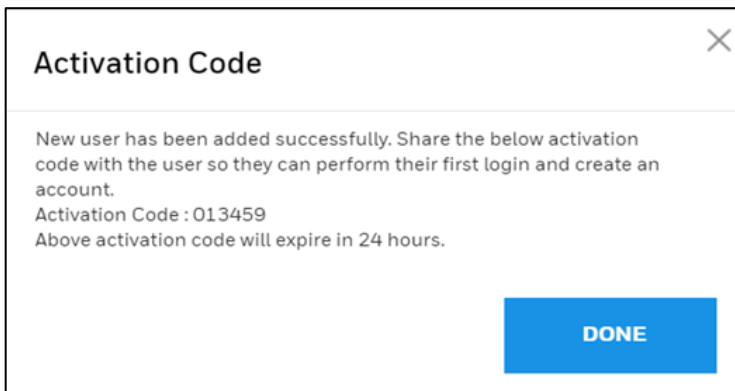


The screenshot shows a modal dialog box titled "Activation Code" with a close button (X) in the top right corner. The message inside reads: "New user has been added successfully. Share the below activation code with the user so they can perform their first login and create an account. Activation Code : 013459. Above activation code will expire in 24 hours." At the bottom right of the dialog, there is a blue button labeled "DONE".

13.10.5 Filter By

There are several ways to filter the list on the screen. Under the column labeled “Filter by”, are selectors for selecting what you see in the columns on the right. Above the filtering options is the number of devices shown.

13.10.5.1 Status

The status of a user can be used as a filter, so that, for example, only active users are included in the list, or only deactivated users are shown. You can clear a status type and associated information by clicking “Clear” or the “X” in the “Status” above the list.

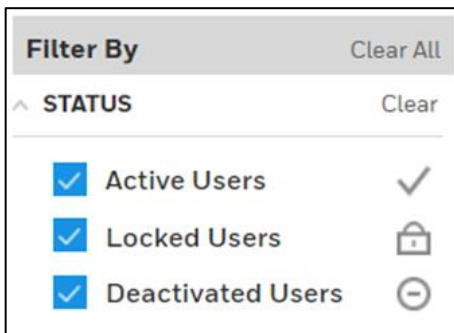

Active Users


An active user is one who is in the current roster of users who can participate in the system’s use, and is associated with a role and an instrument. An active user’s status can be changed to “deactivated” or the user can be deleted from the roster.

Note: If you delete a user, the data cannot be recovered.


Locked Users

As a security feature, if a user tries to log in and provides an incorrect password three times, they are locked out and must contact the administrator to restore access.

When logging in, if an incorrect password is provided twice, this message is shown:

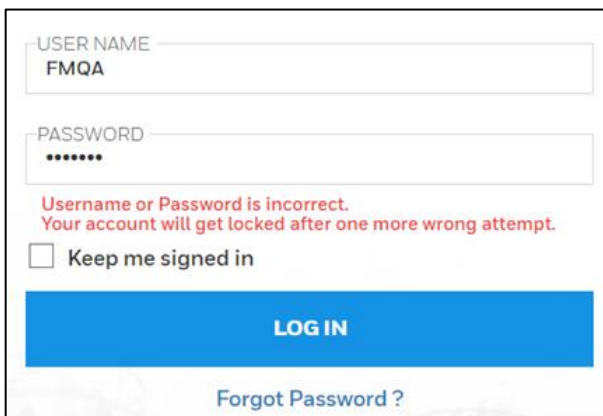


If three attempts are incorrect, then the user is locked out. This message is shown:

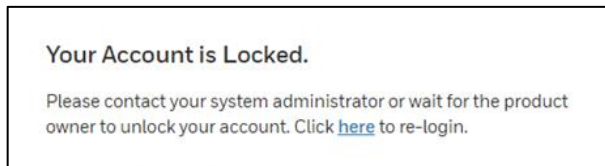

Someone with administrator privileges can unlock the user's status by pulling down the "Actions" menu and clicking "Unlock User."



This message is shown:

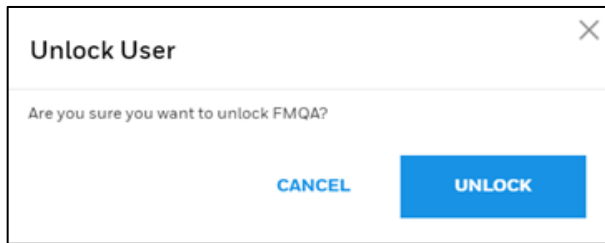

Click "Unlock" to unlock the user's status.

Deactivated Users


A deactivated user has a profile but is not included in the active roster. A deactivated user's status can be changed to "active" or the user can be deleted from the roster.

Note:


If you delete a user, the data cannot be recovered.

13.10.5.2 Name


Search for a user in the User List by name. Either type in a name or select one of the names in the list.

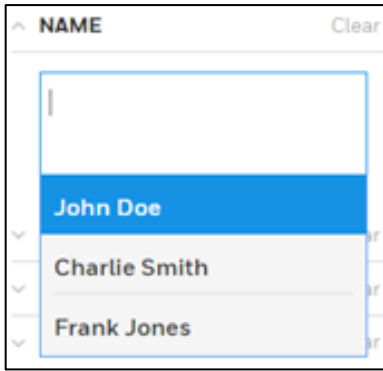

If a match is made, the person's name is then shown in the box:

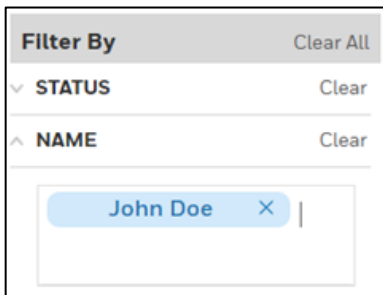


You can add multiple names to the filter by clicking in the box again and selecting a name. The name appears below the previously selected name.

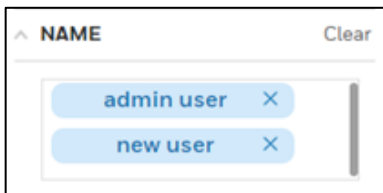

- Click "Clear" to clear all names.
- Click "X" next to a person's name to clear them from the list.

If you type a name and there is no match, then "No matches found" is shown.

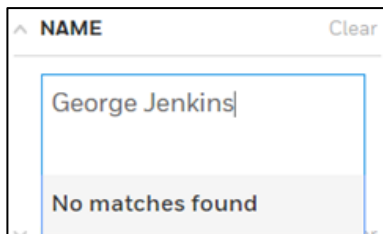

As names are added to the filter, corresponding rows to the right are filled with each person's information. The columns are determined by the Columns setting.

13.10.5.3 Device Assigned

Filter by **devices** that are assigned or unassigned, or to see all (regardless of assignment), click both boxes.

13.10.5.4 User Role

Each user must be assigned one or more roles. Click the appropriate box or boxes.

13.10.5.5 Username

Search by name for a Username in the Username List. Either type in a username or select one of the names in the list.

If a match is made, the username is then shown in the list:

Once you select a username, it shows in the box. It can be cleared by clicking "Clear" or the "X" next to the name.

A selected username is shown above its row of information in the roster.

The screenshot shows a 'User List' interface. On the left, there is a sidebar with navigation icons and a 'Filter By' section. The 'Filter By' section includes:

- STATUS: Clear (with a dropdown arrow)
 - Active Users
 - Locked Users
 - Deactivated Users
- NAME: Clear
- DEVICE ASSIGNED: Clear
- USER ROLE: Clear
- USERNAME: Clear

At the top right, there is a 'Sort by' dropdown menu set to 'Username - Ascending' and a '+' button. Below the filters is a table with the following data:

STATUS	NAME	DEVICE ASSIGNED	USER ROLE	EMAIL	USERNAME	ACTIONS
✓		N	Administrator		administrator	ACTIONS ▾
✓	John Doe	N	Advanced User/Worker	j.doe@honeywell.com	JohnDoe	ACTIONS ▾

13.10.6 Add A User

Click the “+” button to open a page where you fill in information and create the profile for a new user.

The screenshot shows the 'Add a User' form. It features a sidebar with navigation icons and a '+ ' button at the top left. The form includes the following fields:


- * FIRST NAME (40/40 char. remaining)
- MIDDLE NAME (40/40 char. remaining)
- * LAST NAME (40/40 char. remaining)
- EMAIL (email@domain.com, 50 char. remaining)
- * USERNAME (40/40 char. remaining)
- PHONE (30/30 digits remaining)
- ADDRESS1 (150/150 char. remaining)
- ADDRESS2 (150/150 char. remaining)
- CITY (30/30 char. remaining)
- COUNTRY / REGION (dropdown menu)
- STATE / PROVINCE (30/30 char. remaining)
- ZIP CODE (30/30 char. remaining)
- * ROLE (dropdown menu)

 At the bottom right, there are four buttons: CANCEL, DELETE, DEACTIVATE, and ADD. The ADD button is highlighted in blue.

You must provide a First Name, Last Name, and Username, plus you must select a role (or roles). All other information is optional. Once you have provided the necessary information and selected a role, “Add” is highlighted. Click this to add the new user to the roster. If you do not want to save it, click “Cancel.”



After you add a new user, a message is shown that tells you the user must use an activation code during their first login.

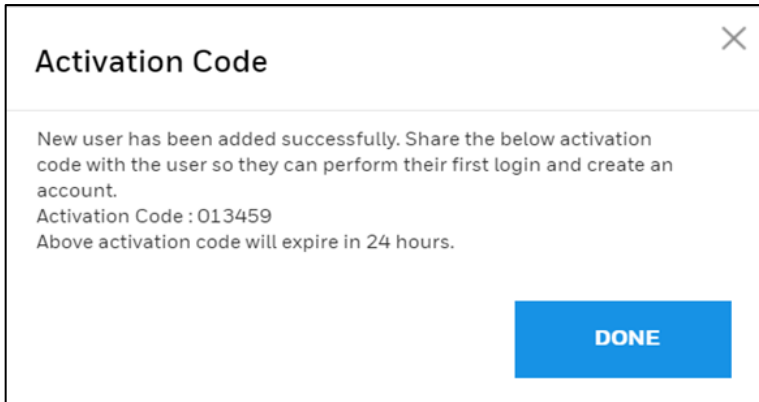


13.10.7 Profile Picture


Click the icon to open the dialog for uploading an image for the profile. The image can be either a .jpg or .png file, but it must be less than 1MB.

To upload an image:

1. Click the blue button.

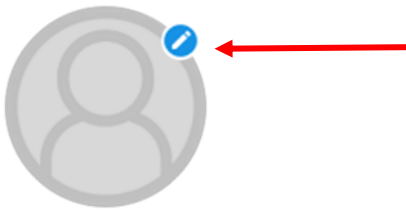

2. Click "Upload Photo."
3. Locate an image on your computer and select it.
4. Click "Open."

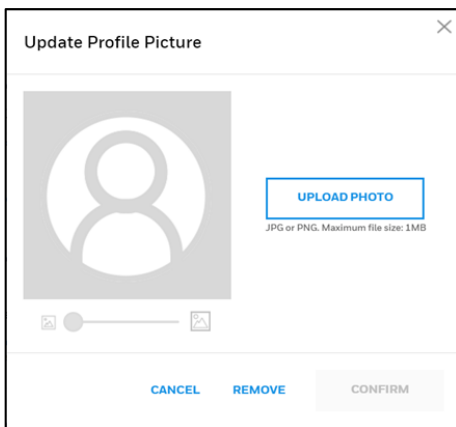

5. When the image appears, move it around with your mouse and/or change its size by adjusting with the slide control.
6. When you are satisfied, click "Confirm"

Note:

Click “Cancel” if you decide not to change the picture, or “Remove” to remove an existing picture.

13.11 Generate Report

Generate a report on a device’s activity by selecting a Report Type, from (start date), To (end date), and Device Serial Number.

Generate Report

REPORT TYPE* ▾

FROM 7/10/2017 → TO 7/17/2017

DEVICE SERIAL NUMBER* ▾

Data Elements

Select a Report Type:

REPORT TYPE* ▾

Event Log

Set your date range.

Note: The maximum date range is one month.

FROM 5/4/2017 → TO 5/11/2017

< APRIL 2017 > < MAY 2017 >

S M T W T F S S M T W T F S

1 1 2 3 4 5 6

2 3 4 5 6 7 8 7 8 9 10 11 12 13

9 10 11 12 13 14 15 14 15 16 17 18 19 20


16 17 18 19 20 21 22 21 22 23 24 25 26 27

23 24 25 26 27 28 29 28 29 30 31

30

DONE

Next, select a device's serial number, followed by the Data Elements you want to include. Two can be selected or de-selected.

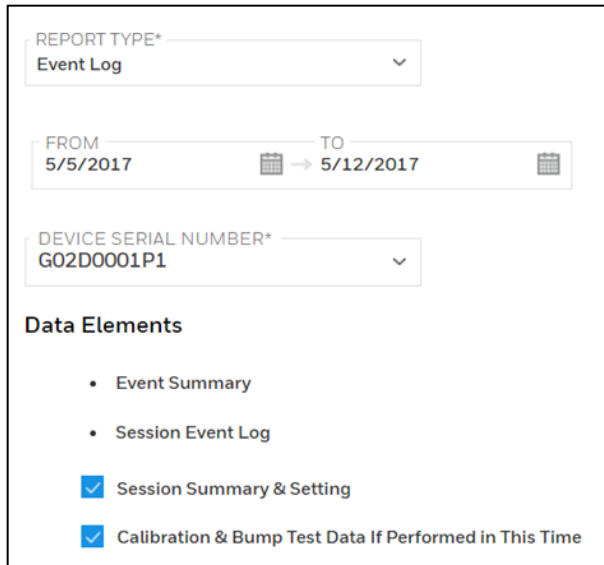

REPORT TYPE*
Event Log

FROM 5/5/2017 TO 5/12/2017

DEVICE SERIAL NUMBER*
G02D0001P1

Data Elements

- Event Summary
- Session Event Log
- Session Summary & Setting
- Calibration & Bump Test Data If Performed in This Time


Click **“Generate”** to create a report based on your criteria.



Note:

If you click “Reset”, it clears all fields.


When the Event Log Report is created, an alert appears, telling you that an event log report has been generated and is available. Click “OPEN” to view it.

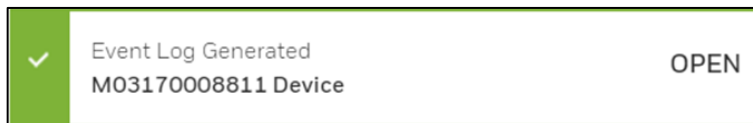

The Event Log Report can be printed or exported to PDF format for later reference, emailing, etc.

Note:

The Event Log Report shows as a single page on the screen, but it is typically longer than one page (the scroll bar along the right side indicates multiple pages' worth of data). Therefore, if you are printing, make sure your printer has adequate paper to accommodate the document.

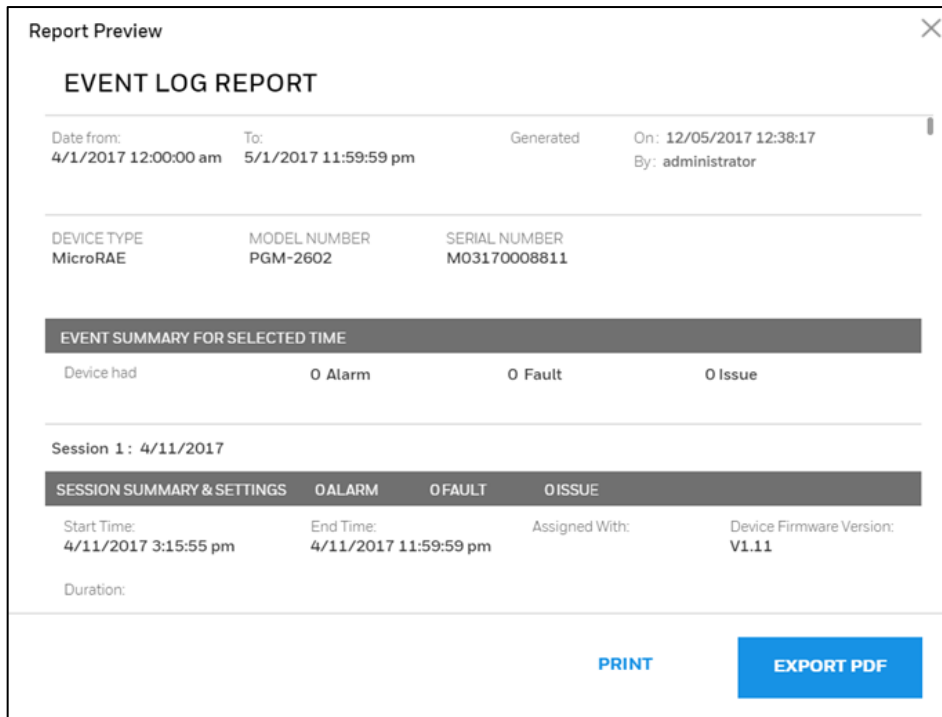


When you are done, click the “X” in the upper right corner to close the window.

13.11.1 Report header


User can add new template (header and logo) to reports. These will appear for all reports.

Follow the below steps to add the new Template and Generate report.

Step 1- Open the Generate report by clicking on Generate Report icon as shown below, click on template to add report header and logo for the report.

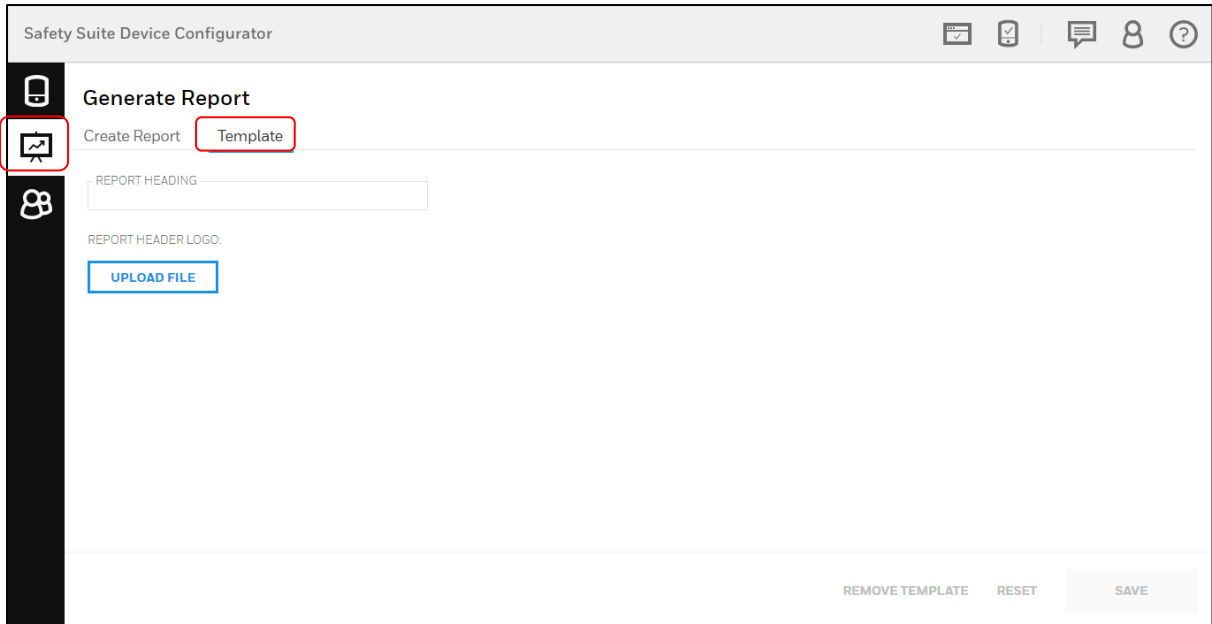

Step 2- Below screen is the example for the new template. Type the **Report Heading** name and click on **CHANGE FILE** to import the Logo, then click on **SAVE** button to save the template.

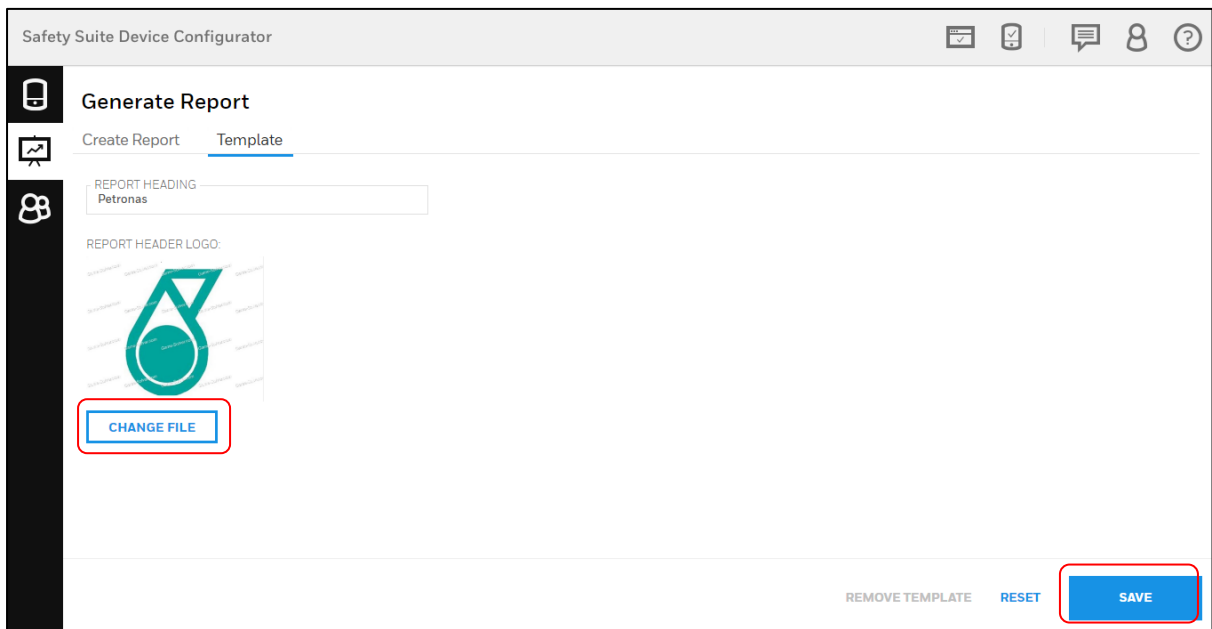

Step 3- To view the logo and header, generate the device report. Click on **Create Report** tab,

- Select the REPORT TYPE by clicking on dropdown.
- Chose the date range and other parameters.


Now click on **GENERATE** option to Generate the report.

The screenshot shows the 'Safety Suite Device Configurator' interface. At the top, there is a title bar with the text 'Safety Suite Device Configurator' and several utility icons (checklist, dropdown, chat, user, help). Below the title bar is a sidebar with three icons: a device, a report, and a user. The main content area is titled 'Generate Report' and has two tabs: 'Create Report' (active) and 'Template'. The 'Create Report' tab contains the following fields and options:

- REPORT TYPE***: A dropdown menu with 'Event Log' selected.
- FROM**: A date field with '01-01-2019' and a calendar icon.
- TO**: A date field with '31-01-2019' and a calendar icon.
- DEVICE SERIAL NUMBER***: A dropdown menu with '5220ULT01181700095' selected.
- Options**: A list of checkboxes:
 - Event Summary
 - Session Event Log
 - Session Summary & Settings
 - Calibration & Bump Test Data if performed in this time

At the bottom right of the form, there are two buttons: a 'RESET' button and a 'GENERATE' button. The 'GENERATE' button is highlighted with a red rectangular border.

Step 4- After clicking on GENERATE, below screen will open with new report. User can PRINT or convert the report to PDF file for the future use.

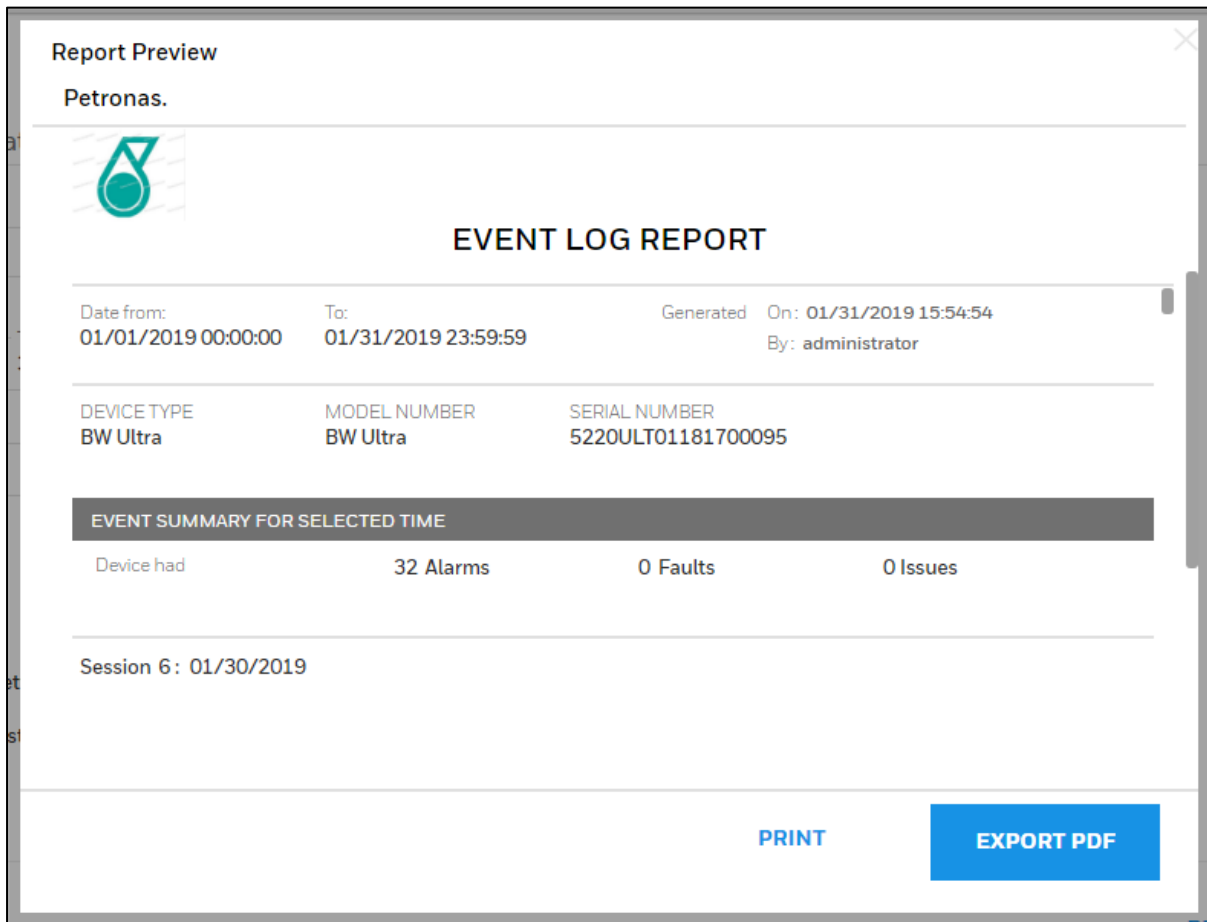


13.11.2 Multidevice reports-Eventlog(Multidevice event report)

User can generate the gas alarm report for the multiple devices.

Below are the steps to follow how to generate multidevice event report.


Step1- Open **Generate report** view in Safety Suite Device Configurator and select the **Create report** option to create the report.

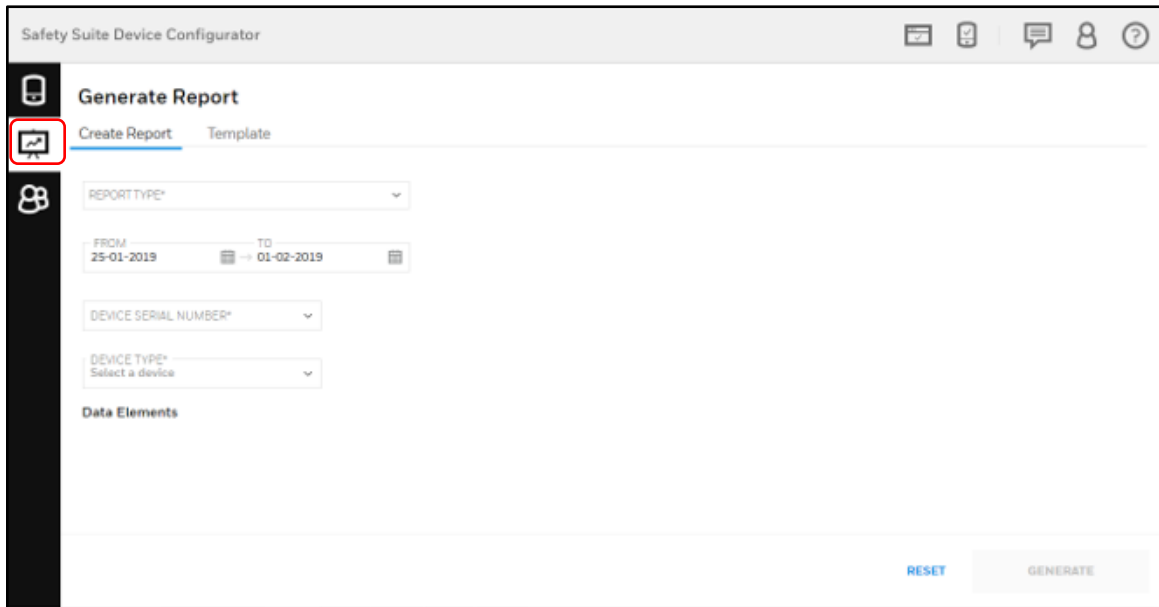


Step 2-To create the report user would need to make the following selection:

- Click on the **REPORT TYPE** dropdown and select “Multidevice Gas Alarm Event Report”
- Select the **FROM** and **TO** date by clicking on calendar option.
- Click on **DEVICE TYPE** and select the device type or select ‘All’.

Now click on GENERATE to continue.

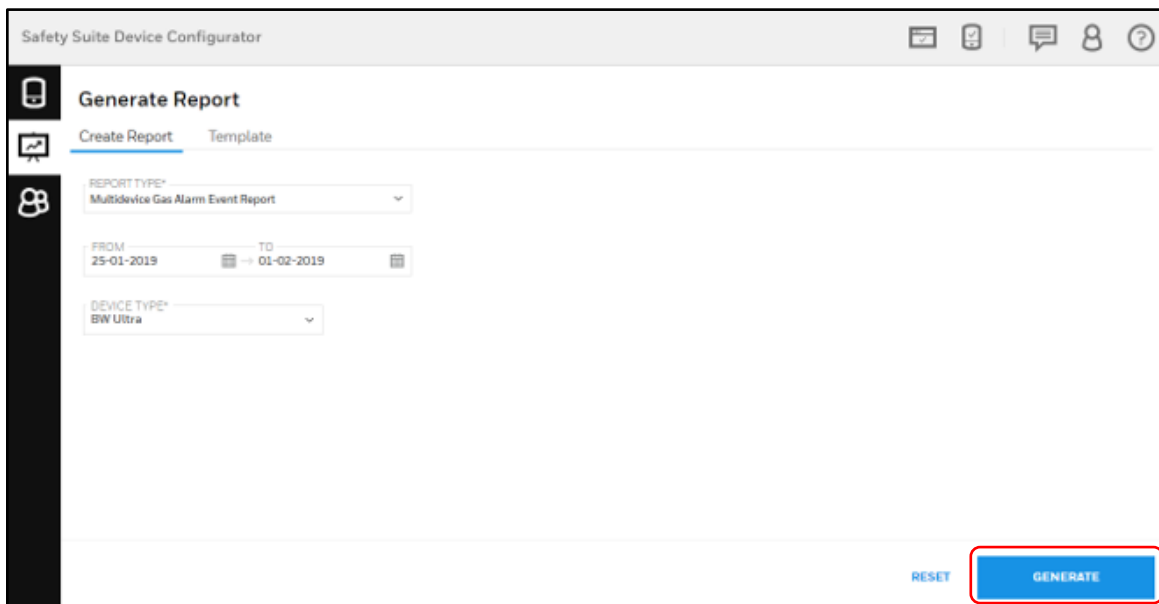


Step 3- After clicking on GENERATE, the report will generate and it shows the notification once report is generated successfully. Then click on OPEN to see the report

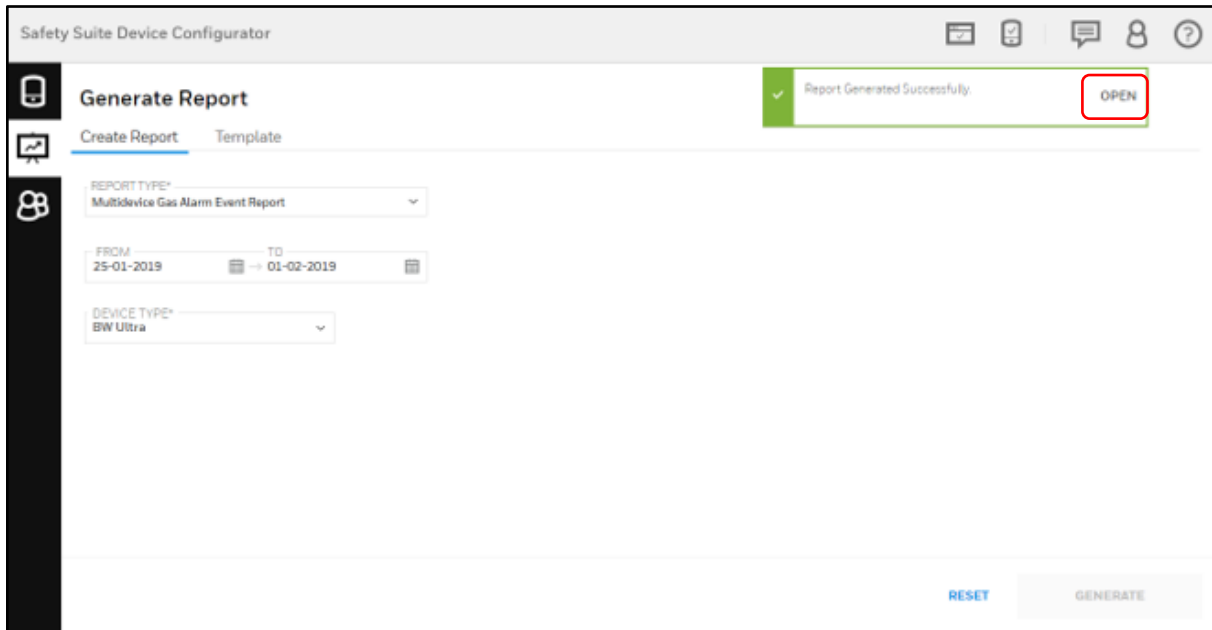

Step 4- Now you can see the Multidevice Gas Alarm Event Report, you can also export the report into PDF or CSV file.

Report Preview

Petronas



Multidevice Gas Alarm Event Report


Data from: 01/25/2019 00:00:00 To: 01/01/2019 23:59:59 Generated On: 02/01/2019 13:24:24

SERIAL NUMBER	START TIME	DEVICE TYPE	DURATION (week)	EVENT TYPE	SENSOR NAME	PEAK VALUE	DEVICE USER
S220_A70118700095	01/05/2019 03:24:05	BW Ultra	30	Low Alarm	O2	19.10	
S220_A70118700095	01/05/2019 03:38:32	BW Ultra	11	Low Alarm	O2	19.28	
S220_A70118700095	01/05/2019 09:20:26	BW Ultra	51	Low Alarm	O2	18.80	
S220_A70118700095	01/05/2019 09:21:58	BW Ultra	28	Low Alarm	O2	18.80	
S220_A70118700095	01/05/2019 09:24:25	BW Ultra	28	Low Alarm	O2	17.45	
S220_A70118700095	01/05/2019 13:28:17	BW Ultra	18	Low Alarm	O2	19.43	
S220_A70118700095	01/05/2019 13:30:11	BW Ultra	22	Low Alarm	O2	19.70	
S220_A70118700095	01/05/2019 13:31:20	BW Ultra	54	Low Alarm	O2	18.40	
S220_A70118700095	01/05/2019 00:28:51	BW Ultra	7	Low Alarm	O2	19.15	

EXPORT PDF EXPORT CSV

14 Uninstall Safety Suite Device Configurator


1. Navigate to All Programs > Honeywell > Safety Suite > Device Configurator and **click** Uninstall Safety Suite Device Configurator to launch the uninstaller for Safety Suite Device Configurator.

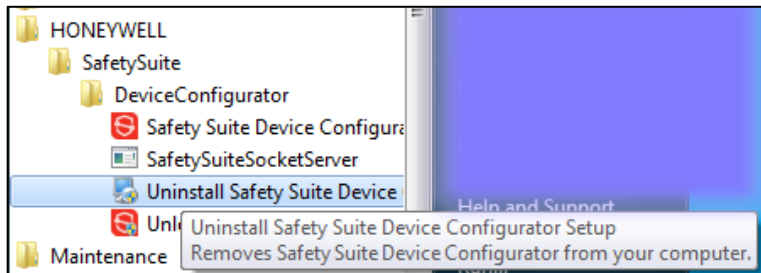


Note:

In Windows 10, follow this path: Start > All Apps > Uninstall Safety Suite Device Configurator

2. Click **Next** on the following screen.

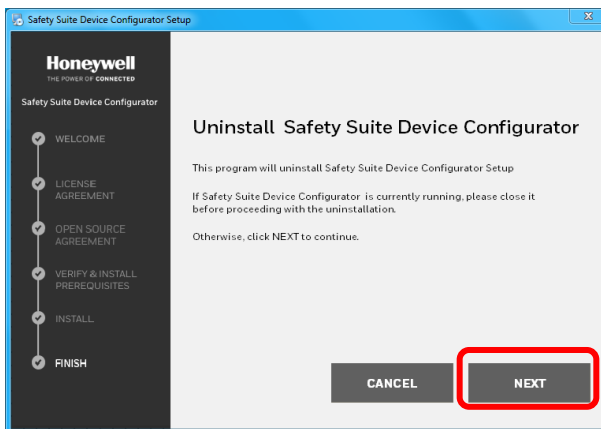

3. Click **Finish** once the installation is complete.

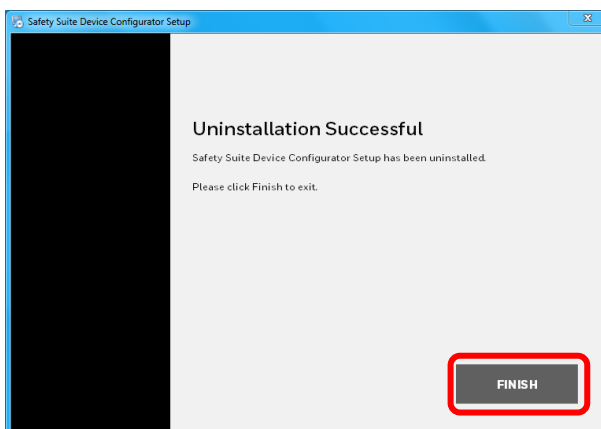


14.1 Delete Instrument Data (Optional)

Perform the following steps only if you plan to delete all instrument data associated with Safety Suite Device Configurator. Once these steps are performed, the data cannot be recovered.

14.1.1 Uninstall Microsoft SQL Server 2012


1. Navigate to Control Panel > Programs and Features, and double-click “Microsoft SQL Server 2012”:

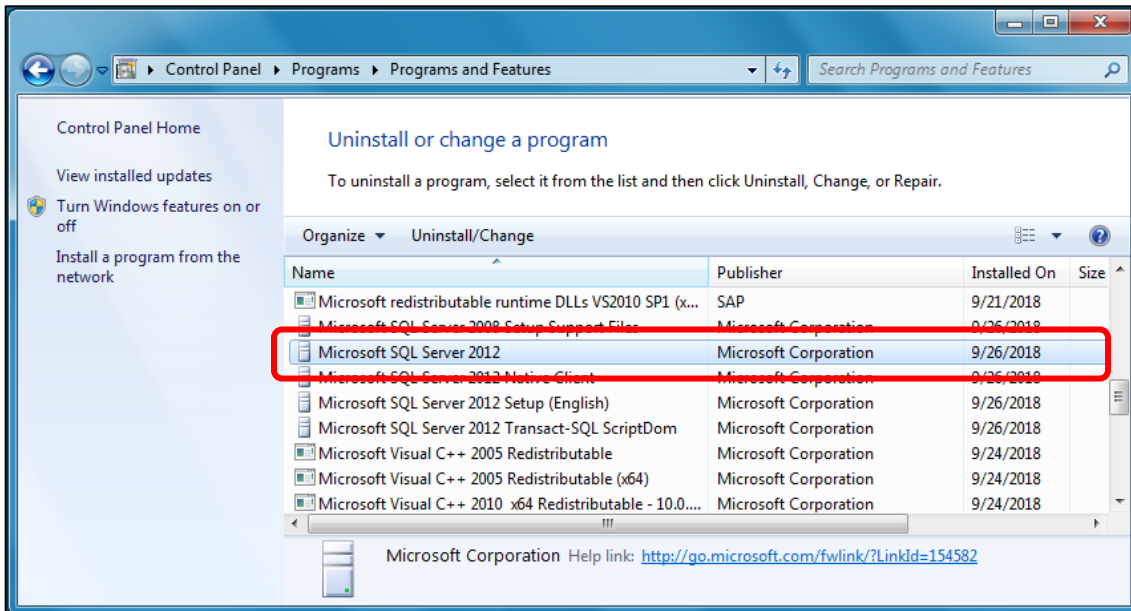


2. Click **Remove** to initiate the removal of Microsoft SQL Server 2012:




3. When the next screen is shown, click **OK**:

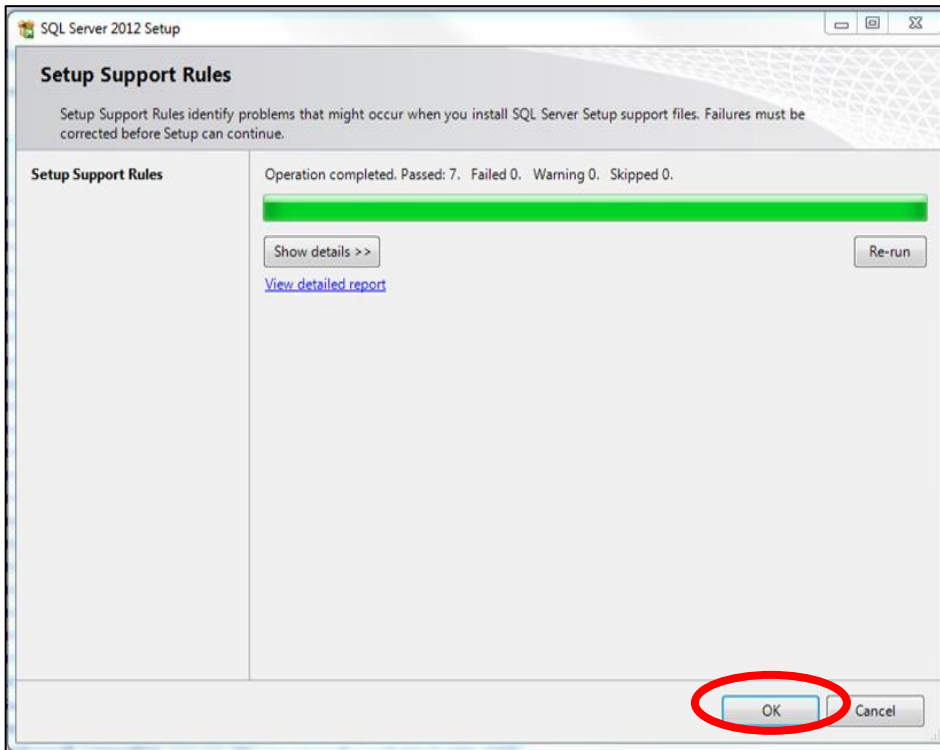


4. **Select** Safety Suite Device Configurator from the drop-down menu, and click **Next**:

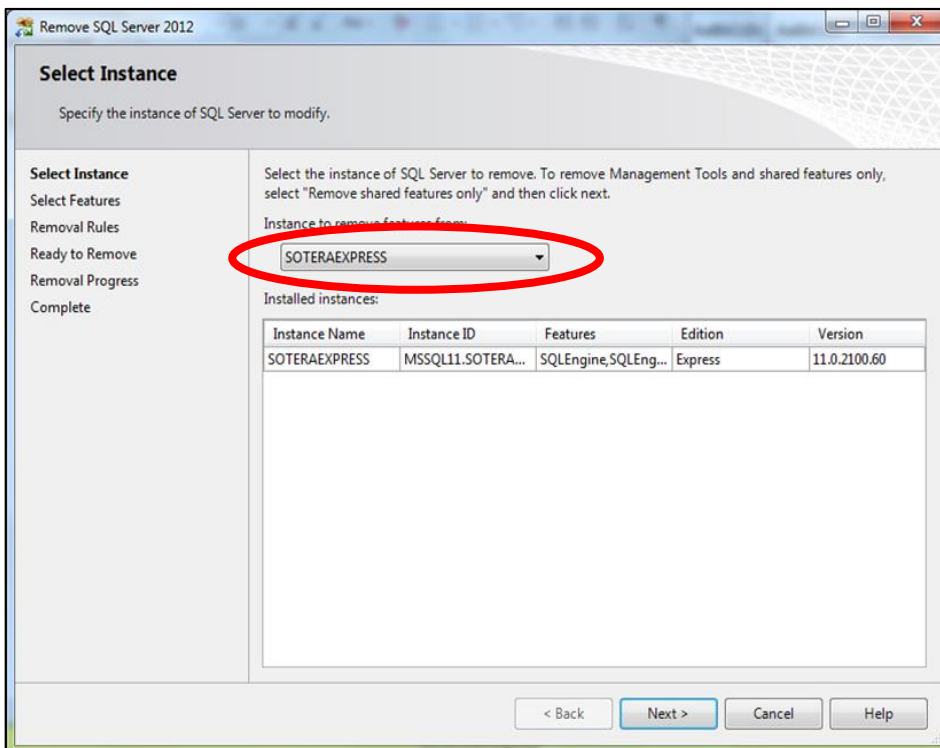


5. Click **Select All** followed by **Next**:

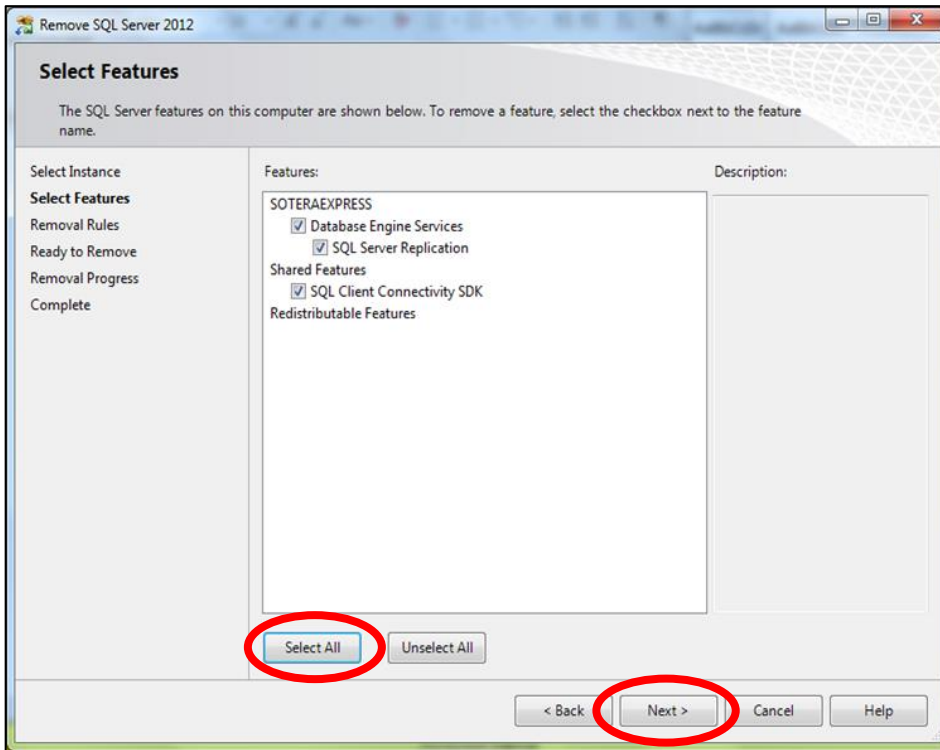


6. When the new screen appears, click **Next**:

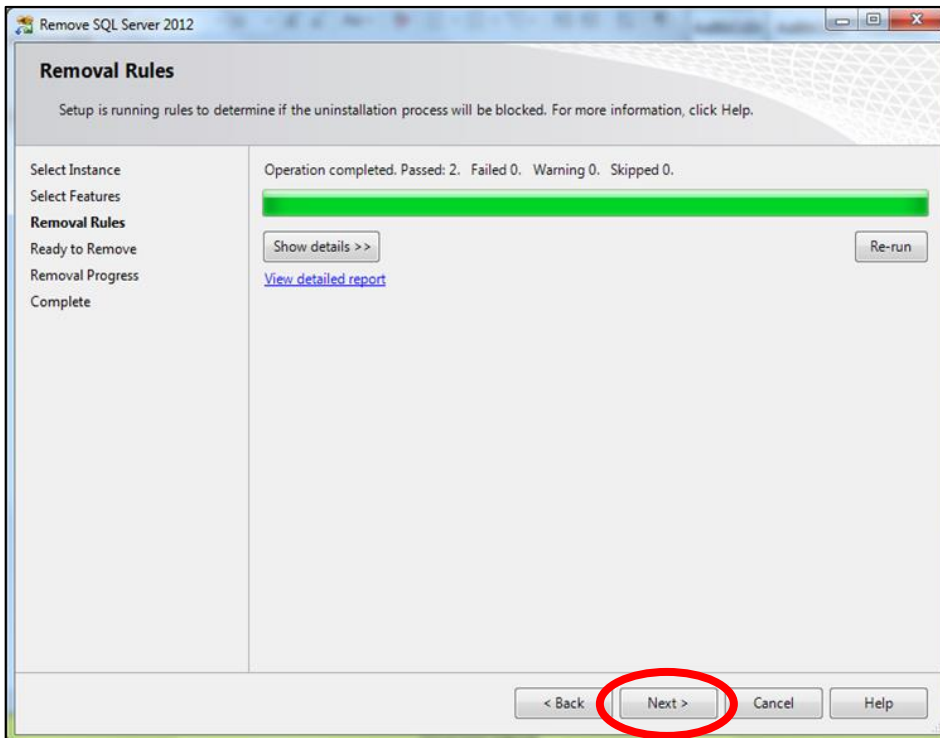


7. Click **Remove**:

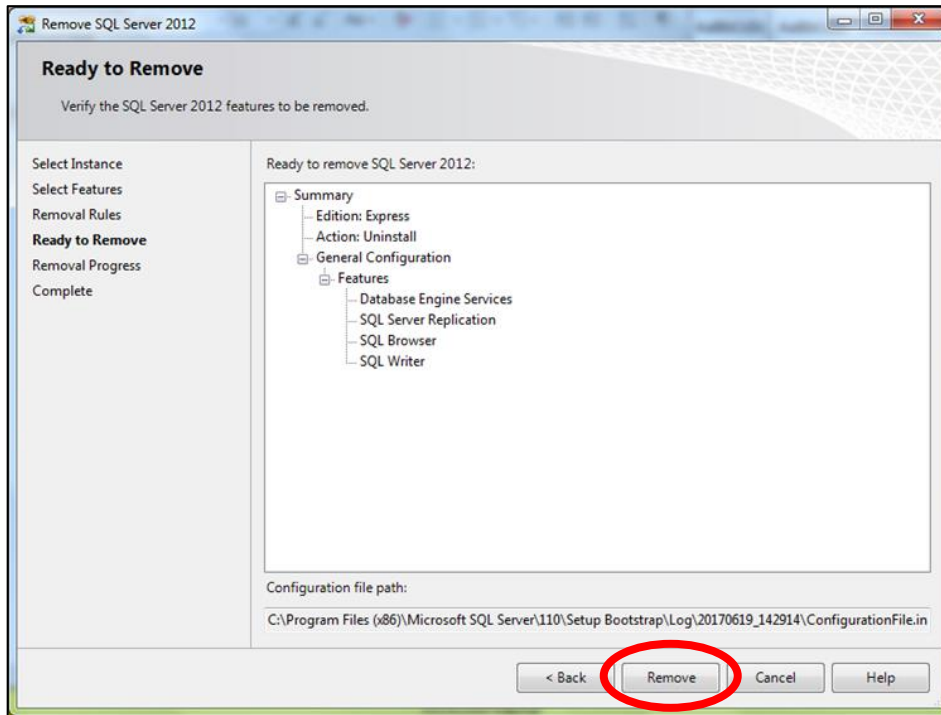


8. The removal progress is shown by a progress bar:

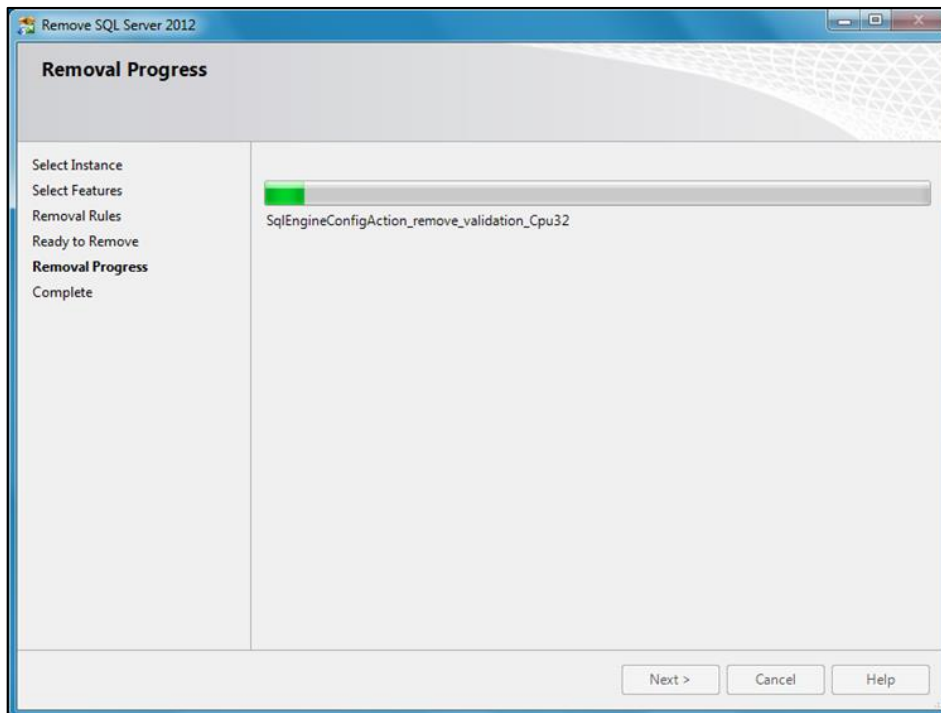

9. Click **Close** to complete the removal of the Microsoft SQL Server instance:

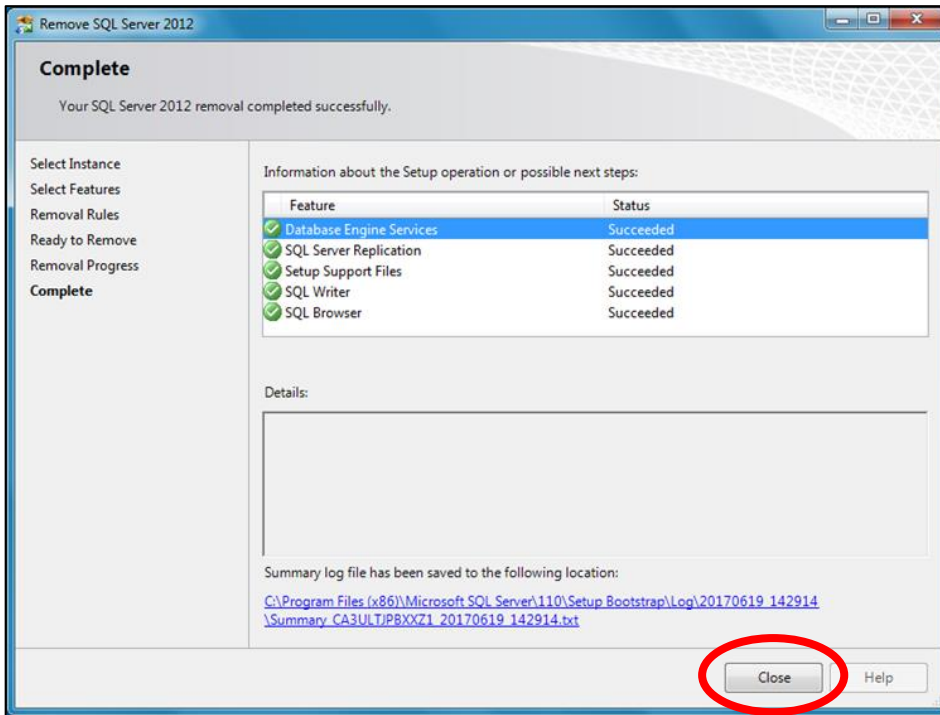

10. Finally, **delete** the folder Mssql11.Soteraexpress. Go to C:\Program Files (x86) \Microsoft SQL Server, and delete the folder:

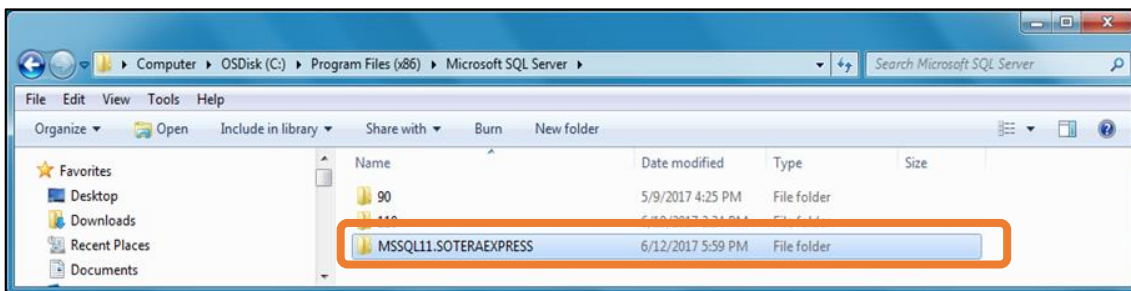


15 Migrating ProRAE Studio Database to Safety Suite Device Configurator

You can migrate your existing ProRAE Studio database to Safety Suite Device Configurator. This database contains historical data about RAE instruments.

IMPORTANT!


You must install Safety Suite Device Configurator before you perform the transfer.

1. Identify ProRAE Studio database folders for migration and copy those folders to the system where Safety Suite Device Configurator is installed.
2. Log into Safety Suite Device Configurator. The first time you do this, the screen shown here will appear:

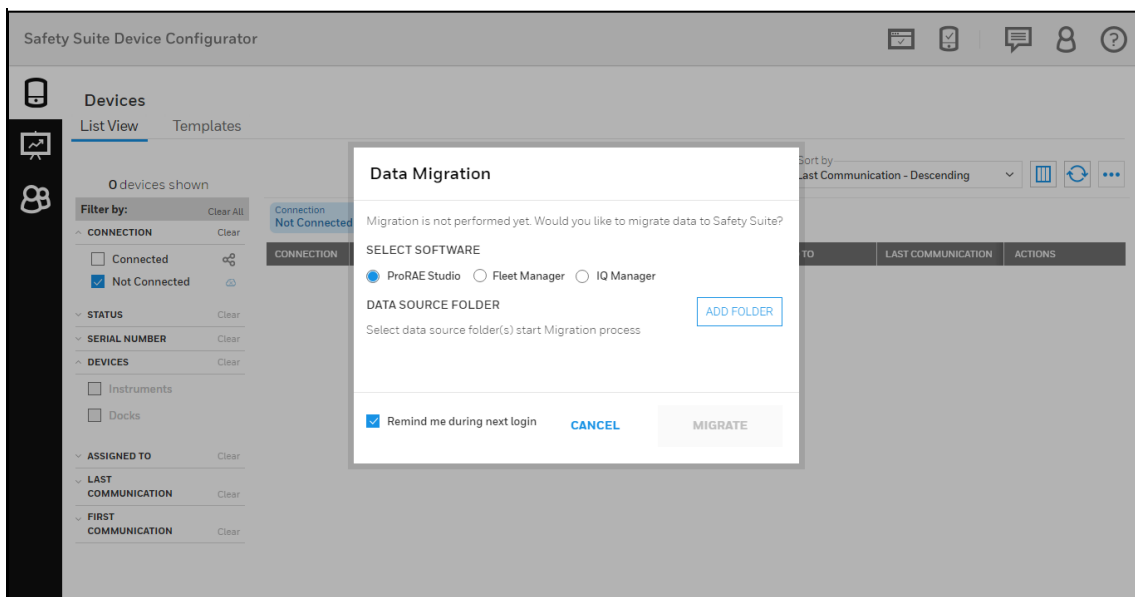


Note:

This dialog is shown every time you log in until the migration is performed. If you do not want to see this message, uncheck the option labeled "Remind me during next login". At the next login, under "Administrator", select "Data Migration" from the menu and follow the instructions in the dialog box:

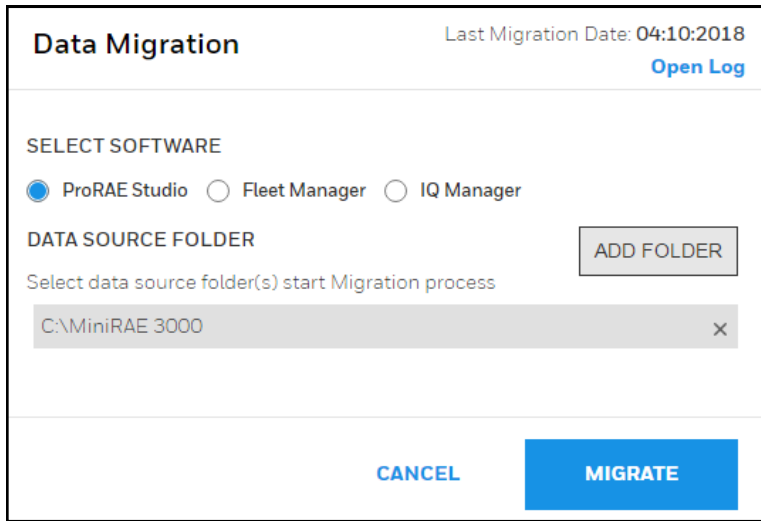


3. Where it says, “Select Software,” select ProRAE Studio.
4. At “Data Source Folder,” click “Add Folder.”
5. Locate the database folder for ProRAE Studio (folders with .prs files) and select it.
6. Click “Migrate” to begin migration. During the migration process, this progress message appears on the screen:

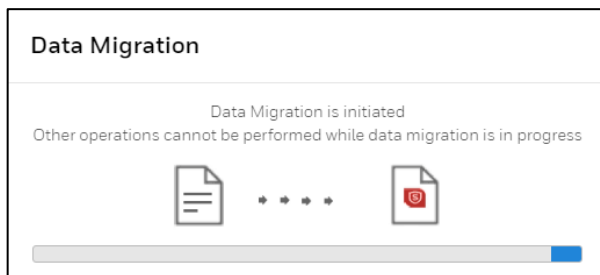


IMPORTANT!

Do not interrupt the migration. Depending on the size of the database being imported, the process can take from a few minutes to a few hours.

When the migration is completed successfully, a summary box is shown:

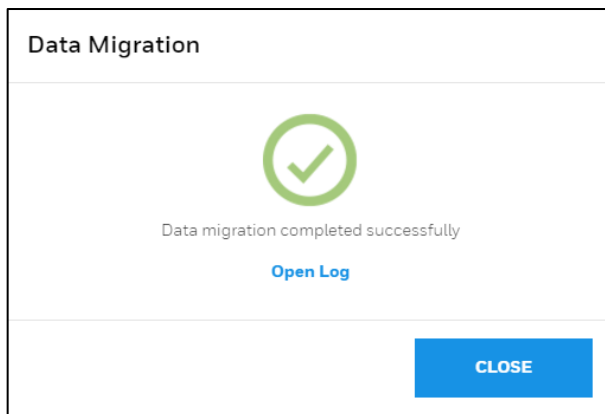

If the data migration fails, this message is shown:

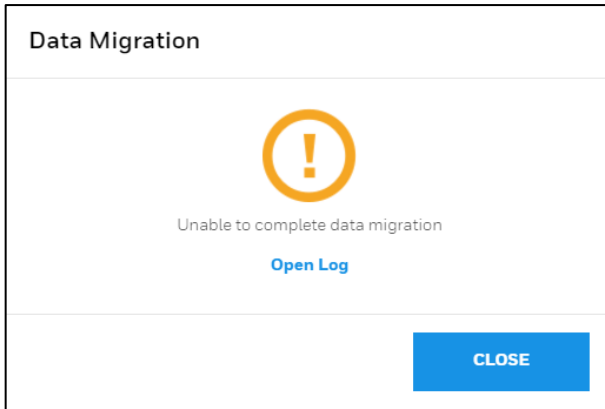

If you want to view diagnostic logs for the migration, click “Open Log.”


16 Migrating Fleet Manager Database to Safety Suite Device Configurator

You can migrate your existing Fleet Manager database to Safety Suite Device Configurator. This database contains historical data about the instruments.

IMPORTANT!


You must install Safety Suite Device Configurator before you perform the transfer.

7. Identify Fleet Manager database folders for migration and copy those folders to the system where Safety Suite Device Configurator is installed.
8. Log into Safety Suite Device Configurator. The first time you do this, the screen shown here will appear:

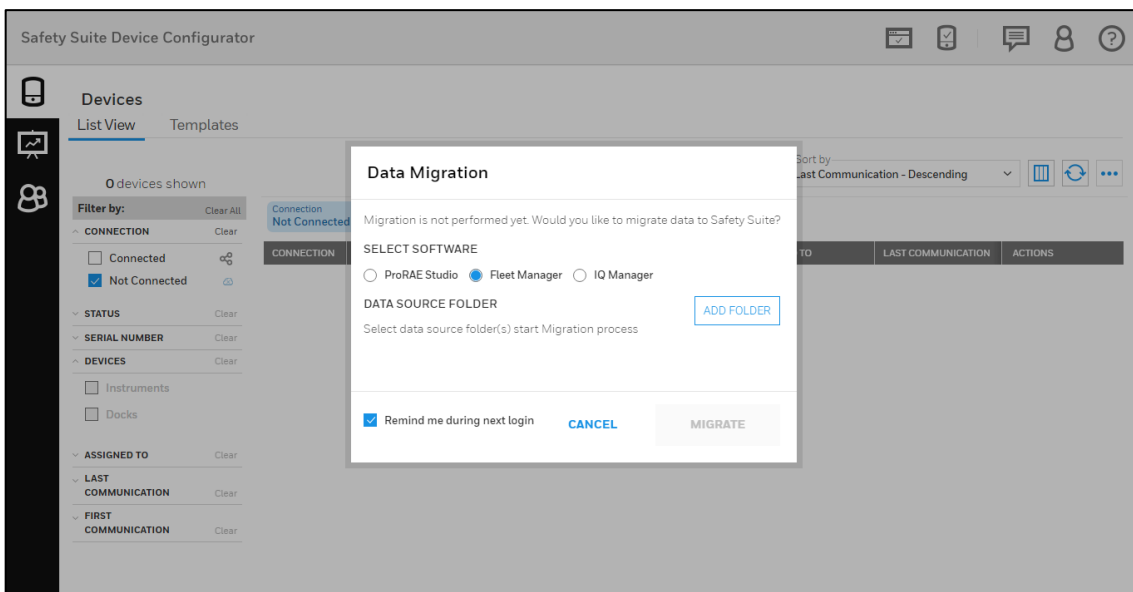


Note:

This dialog is shown every time you log in until the migration is performed. If you do not want to see this message, uncheck the option labeled “Remind me during next login.” At the next login, under “Administrator,” select “Data Migration” from the menu and follow the instructions in the dialog box:

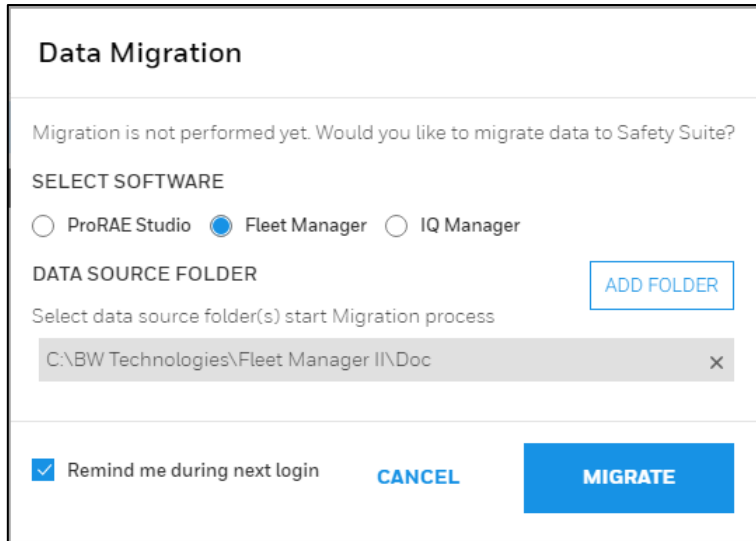


9. Where it says, “Select Software,” select Fleet Manager.
10. At “Data Source Folder,” click “Add Folder.”
11. Locate the database folder for Fleet Manager and select it.
12. Click “Migrate” to begin migration. During the migration process, this progress message appears on the screen:

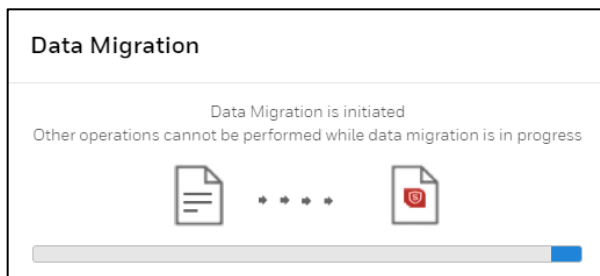


IMPORTANT!

Do not interrupt the migration. Depending on the size of the database being imported, the process can take from a few minutes to a few hours.

When the migration is completed successfully, a summary box is shown:

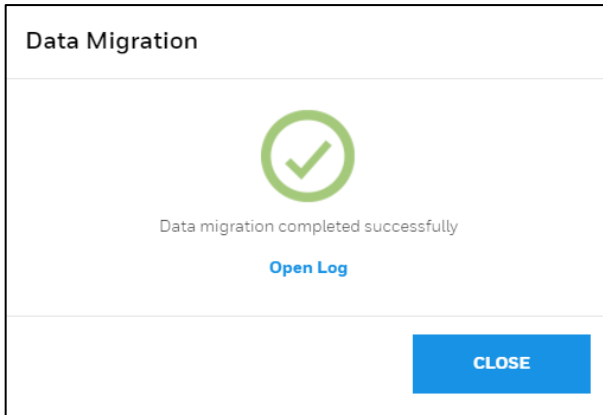

If the data migration fails, this message is shown:

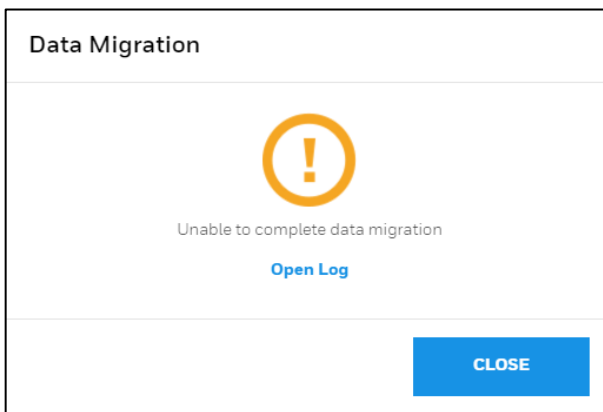

If you want to view diagnostic logs for the migration, click “Open Log.”

Notes:

After successful database migration, you are now able to view details for Gas Alert Micro Clip and BW Clip instrument data in the database.

Safety Suite Device Configurator accepts the Fleet Manager Databases created using Fleet Manager version v4.4.2. Any databases created using Fleet Manager versions prior to this must first be upgraded using Fleet Manager.


17 Migrating IQ Manager Database to Safety Suite Device Configurator

You can migrate your existing IQ Manager database for ToxiPro devices to Safety Suite Device Configurator. This database contains historical data about the instruments.

IMPORTANT!


You must install Safety Suite Device Configurator before you perform the transfer.

1. Log into Safety Suite Device Configurator. The first time you do this, the screen shown here will appear:

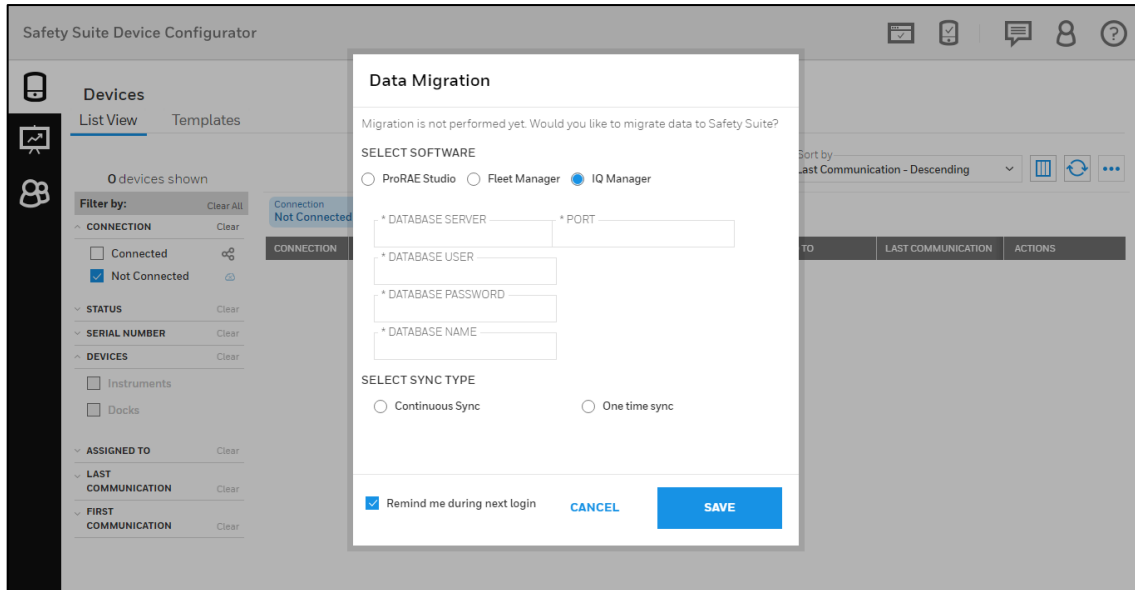

Note:

This dialog is shown every time you log in until the migration is performed. If you do not want to see this message, uncheck the option labeled “Remind me during next login.” At the next login, under “Administrator,” select “Data Migration” from the menu and follow the instructions in the dialog box:

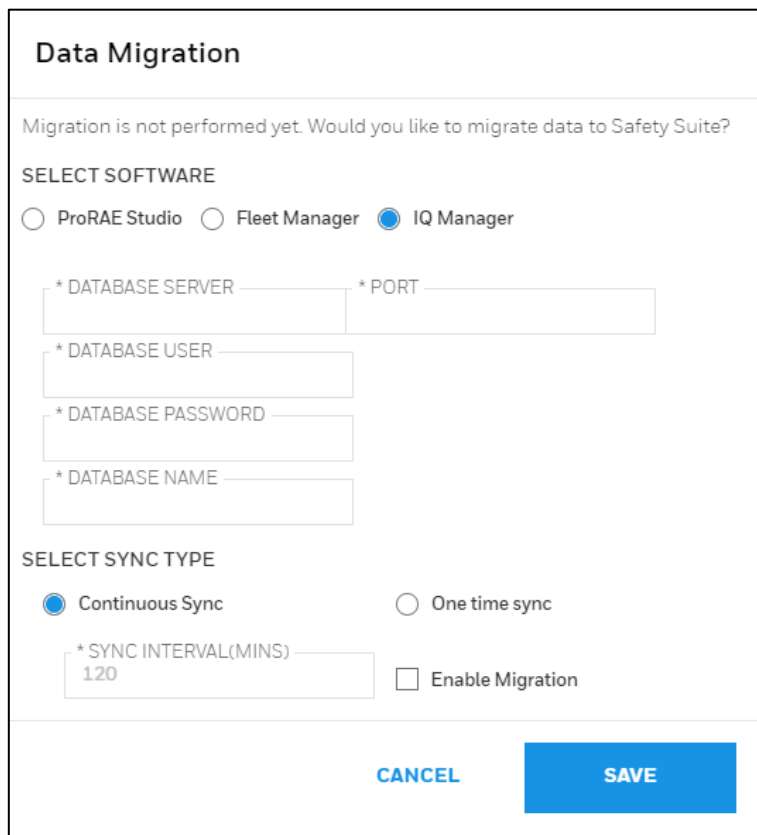

2. Where it says, “Select Software,” select IQ Manager.

3. Provide the “Database Server IP/Name”, “Port number” (5432 is the default Port), “Database User Name”, “Database Password”, “Database Name”.
4. Select the “Continuous Sync” in Sync type section.
5. Select “Sync Interval time” in minutes.
6. Click “Enable Migration”.
7. Click “Save” to begin migration.

IMPORTANT!

Depending on the size of the database being imported, the process can take from a few minutes to a few hours.

Notes:

After successful database migration, you are now able to view ToxiPro instrument data in the database.

17.1 Backup of Source Files


After completion of migration, the source files are available in this folder:

In case the Fleet Manager database includes data for instruments other than BW Clip or Gas Alert Micro Clip, do not delete these files.

18 Migrating IQ Manager Database to Safety Suite Device Manager

You can migrate your existing IQ Manager database for ToxiPro devices to Safety Suite Device Manager. This database contains historical data about the instruments.

1. Log into Safety Suite Device Manager. The first time you do this, the screen shown here will appear:

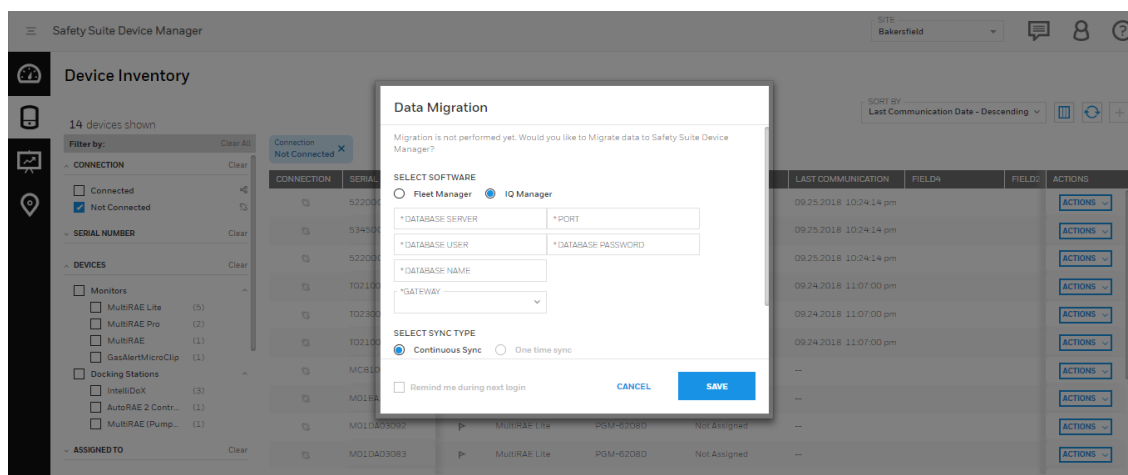

1. Where it says, “Select Software,” select IQ Manager.
2. Provide the “Database Server IP/Name”, “Port number” (5432 is the default Port), “Database User Name”, “Database Password”, “Database Name”.
3. Select the “Continuous Sync” in Sync type section.
4. Select “Sync Interval time” in minutes.
5. Click “Enable Migration”.
6. Click “Save” to begin migration.
7. Migration process will continue in the background based on the sync interval specified.

Notes:

After successful database migration, you are now able to view ToxiPro instrument data in the inventory page.

19 Device Configurator FAQs

19.1 General Questions

- **Do I have to purchase Honeywell Safety Suite Device Configurator before I can use it?**

Honeywell Safety Suite Device Configurator is offered free of charge to all Honeywell customers who purchase Honeywell Gas instruments.

- **What are the minimum software and hardware requirements for Honeywell Safety Suite Device Configurator?**

Hardware

- CPU, 1.0 GHz or higher
- A. ○ Color monitor (1366x768 or higher resolution or higher, 16-bit color)
- 2 GB RAM
- 4 GB of free hard disk space
- USB port for instrument/dock connection
- LAN connection for network-connected docks

Software

- Microsoft Windows 7 SP1 (32 bit/64 bit) or Microsoft Windows 10 (64 bit)
- .Net Framework v4.6.1 or above

- **Does Honeywell Safety Suite Device Configurator support data migration for Fleet Manager II, ProRAE Studio II and IQ Management Software Suite?**

Honeywell Safety Suite Device Configurator supports data migration from Fleet Manager II for all the supported instruments. In addition, it supports data migration for GasAlert Extreme. Existing Fleet Manager II instances should be upgraded to the latest version before initiating data migration. The software also supports data migration from ProRAE Studio II for all supported RAE instruments. Data migration from IQ Management Software Suite is Supported for ToxiPro.

- **Can Honeywell Safety Suite Device Configurator manage both BW & RAE Systems instruments?**

Yes, Honeywell Safety Suite Device Configurator is a single software solution designed to support both BW & RAE Systems instruments and manage these devices through a common interface and a central data repository which resides on the local system.

- **What instrument connectivity options are currently supported by Honeywell Safety Suite Device Configurator?**

Honeywell Safety Suite Device Configurator currently supports instrument connectivity

- A. through IntelliDoX, MicroDock II and AutoRAE 2 for BW & RAE Systems instruments. BW Instruments can connect directly through IR Dongle wherever applicable. RAE instruments can also connect directly through the Travel Charger.

➤ **What instruments are supported by Honeywell Safety Suite Device Configurator?**

The following is a list of currently supported instruments.

IntelliDoX & MicroDock II

- BW Clip & BW Clip Real Time
- BW MicroClip XL & BW MicroClip X3 IntelliDoX
- BW Clip4
- BW Solo
- A. ○ BW Ultra MicroDock II
- BW MaxXT II
- BW Quattro
- GasAlertMicro 5

IR Dongle

- BW MaxXT II
- BW MicroClip XL & BW MicroClip X3
- BW Quattro
- BW Ultra

AutoRAE 2 & Travel Charger

- MicroRAE
- MiniRAE 3000 & MiniRAE Lite
- MultiRAE Family (Benzene & Wing Tank model support in future releases)
- ppbRAE 3000
- QRAE 3
- ToxiRAE Pro Family
- Ultra 3000

Direct USB

- AreaRAE Plus & AreaRAE Pro

➤ **Does Honeywell Safety Suite Device Configurator require administrative privileges on the windows operating system?**

Yes, Honeywell Safety Suite Device Configurator does require administrative privileges on the operating system.

➤ **What Fleet Manager features are not supported by Honeywell Safety Suite Device Configurator?**

Honeywell Safety Suite Device Configurator has streamlined the tasks performed by Fleet Manager and greatly improves the overall user experience. However, it does not

- A. support user- defined fields and custom reporting features of Fleet Manager.

➤ **What should I do when Device Configurator does not respond?**

A.

Try to sign out and close the application. If does not work, kill the application using Task Manager from the taskbar.

➤ **Does Device Configurator work without Internet connection?**

Device Configurator works without Internet connection. Automatic Firmware upgrade does not work without Internet connection, user must select the firmware file to upgrade the firmware.

A.

➤ **Where can I find Device Configurator user guide/ help document?**

Help document is available the Device Inventory page. After login, you can see a question icon on right corner of the top header, click on the icon and click on the “Help” to

A. see the help document.

19.2 Installation

➤ **What all Windows version are supported for Device Configurator?**


A. Device Configurator supports Windows 7(32bit,64bit) and Windows 10(64 bit).

➤ **How to troubleshoot sql server issue during Device Configurator installation?**

Please the steps for SQL server installation related issues.


- Go to user's temp directory to get sql.exe.
- This will look like C:\Users\<(userid)\AppData\Local\Temp

A.

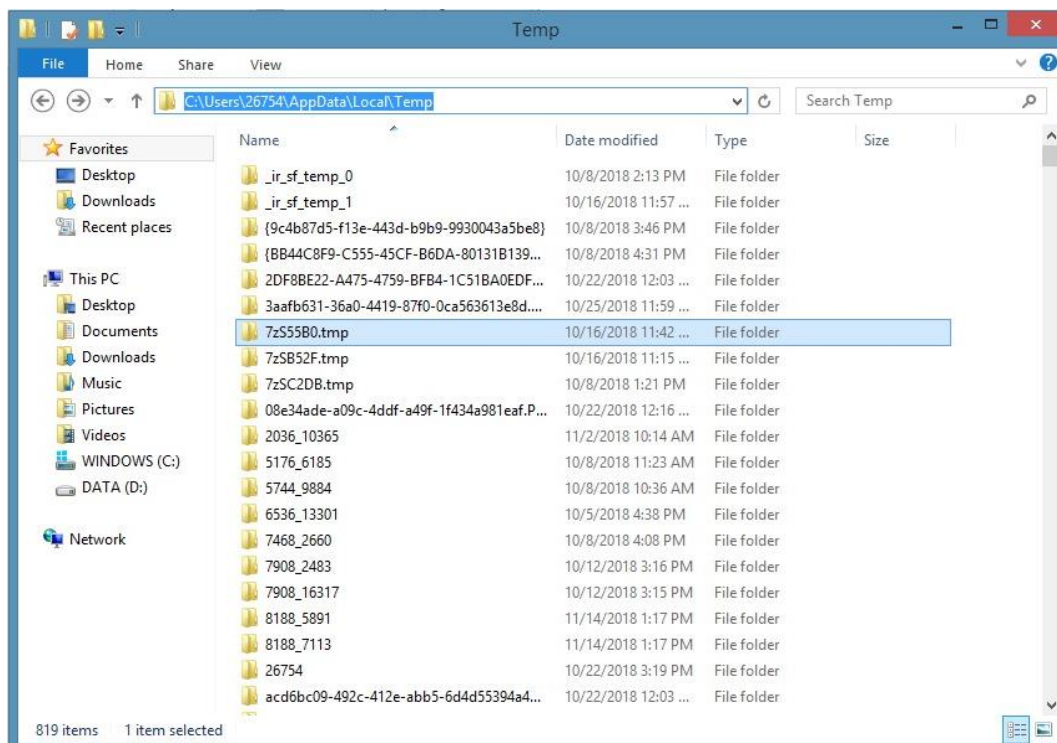


A.

- Click on file with 7zxxxxxx.tmp and it will open below screen

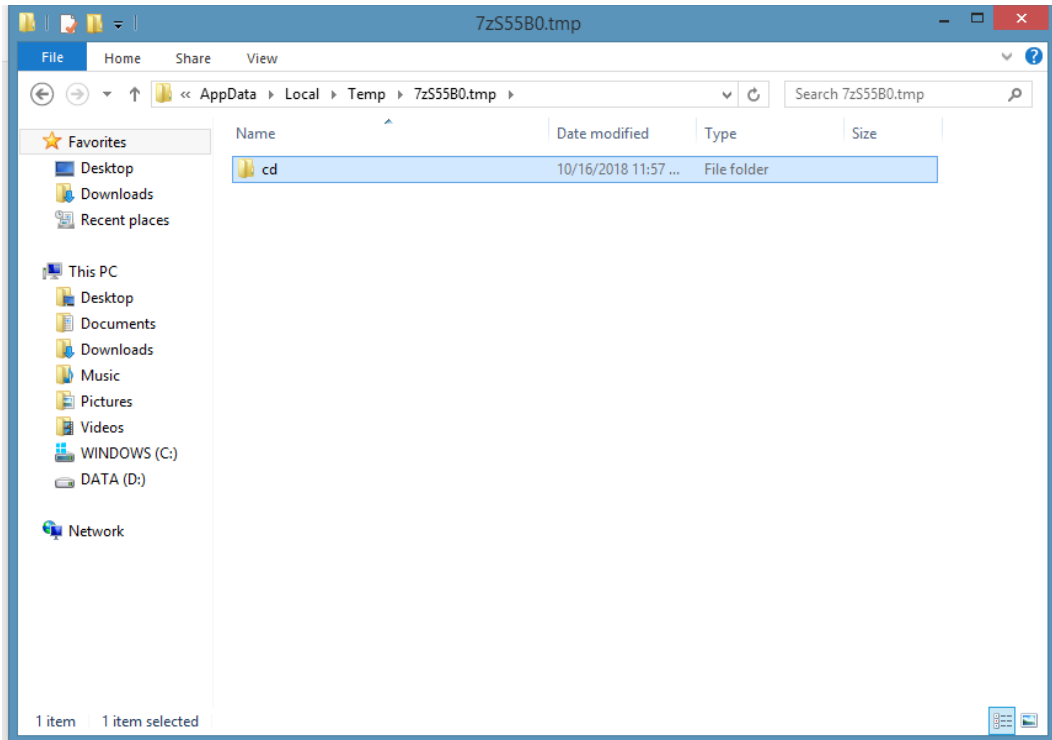


- Click on CD folder and will open below screen. Copy the path by clicking on the folder at address bar.
- It will be looks like `C:\Users\XXXX\AppData\Local\Temp\7zS55B0.tmp\cd`

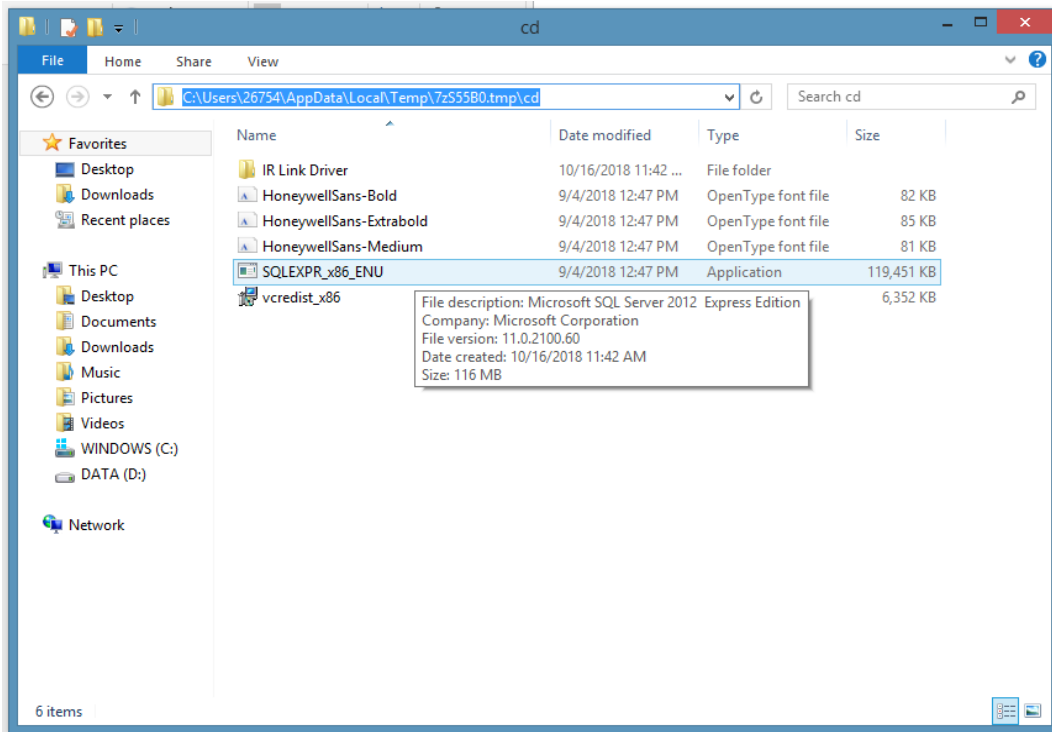


- Open command prompt as administrator and copy the sql path in cmd screen and hit enter:

- o cd C:\Users\xxxxxx\AppData\Local\Temp\7zS2286.tmp\cd

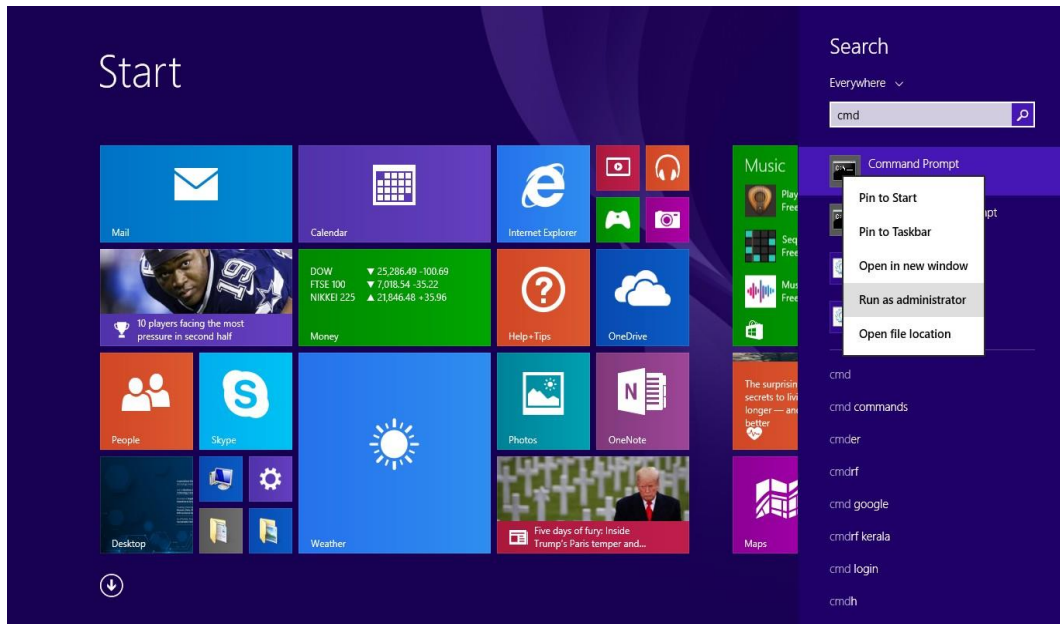

- o After hitting enter button, cmd screen looks like below image.

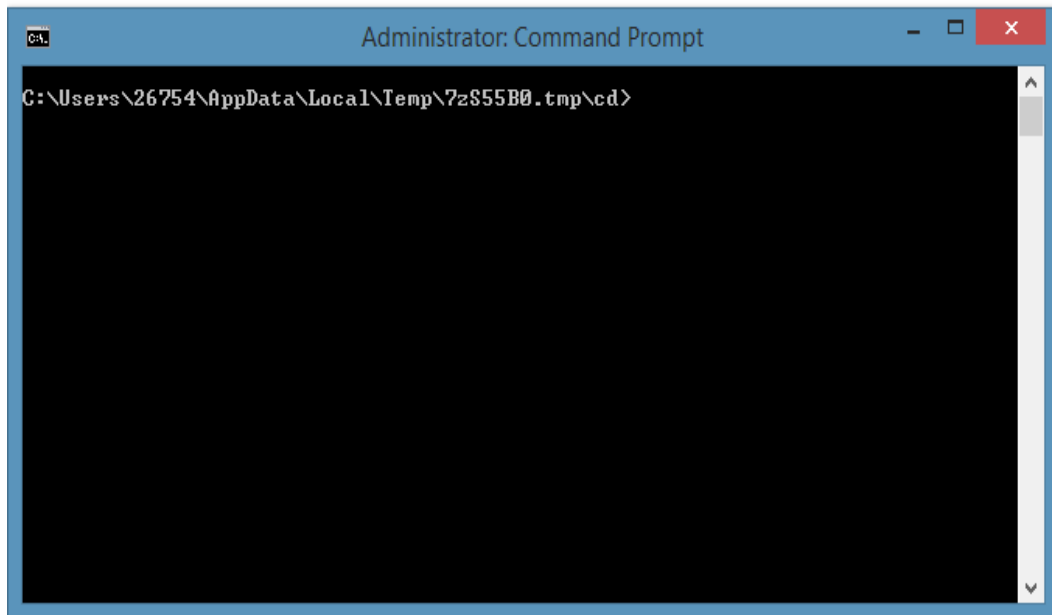

- o Copy the blow line and paste in cmd screen to uninstall SQL package completely.
- o SQLEXPRESS_x86_ENU.exe /ACTION="unInstall"
/INDICATEPROGRESS="TRUE"/FEATURES=SQLENGINE,
REPLICATION,FULLTEXT,BIDS,CONN,IS,BC,SDK,BOL,SSMS,ADV_SSMS

```
Administrator: Command Prompt
C:\Users\26754\AppData\Local\Temp\7zS55B0.tmp\cd>SQLEXP_x86_ENU.exe /ACTION="uninstall" /INDICATEPROGRESS="TRUE" /FEATURES=SQLENGINE, REPLICATION, FULLTEXT, BIDS, CONN, IS, BC, SDK, BOL, SSMS, ADU_SSMS
```

- After copying the above line to cmd press enter button, this will uninstall package completely.
- if any errors are coming continue with uninstallation and after that run the above command again.
- To make sure all files removed, go to below path and delete all folders at - C:\Program Files (x86)\Microsoft SQL Server

Yes. Both can be installed on same machine. While installing DM over DC, if you encounter error that BW Device is already running then click on retry and continue with installation.

➤ **What all Honeywell Device Application should not be running when using Device Configurator?**

Fleet Manager, ProRAE Studio, IQ Manager and ProRAE Guardian can be installed but should not be running when using Device Configurator.

➤ **What should I do when I see notification to reboot my machine repeatedly?**

It means that SQL server is not installed properly and there is some issue in installing SQL server. Please refer the question for SQL installation related issue.

➤ **How to troubleshoot sql server issue during Device Configurator installation?**

➤ **Device Configurator installed SQL server for its back-end database, is it possible to use a database on a shared server rather than a localized one on the PC?**

A. The software is designed for local use on a PC. Each PC needs its own local copy.

➤ **Device Configurator IIS does that mean the functions of the software are available via a webpage or does each PC that uses Fleet Manager need this software installing?**

The software is designed for local use on a PC. Each PC needs its own local copy.

A.

- **The pre-requisites imply Device Configurator is a desktop app, but could this run on a server?**

It should most likely be able to run on server. However, we have certified it only on Windows 7 & Windows 10.

- **How to deploy Device Configurator in a Firewalled environment? If they all use the installed SQL server database how would multiple installs work?**

Each install uses its own SQL instance. You cannot share on SQL instance across multiple installs.

A.

- **What happens if I do not create password immediately after the installation?**

When user login next time, it'll ask to create password.

19.3 Login

- **I have installed Device Configurator but not able to login. What should I do?**

A) Check the mentioned services are running, Open Services.msc in run window.

- A.
 - SafetySuite.DCBWDeviceService
 - SafetySuite.DCDatabaseService
 - SafetySuite.DCMainService
 - SafetySuite.DCRAEDeviceService
 - SQL Server (SOTERA EXPRESS)

A. If not Please restart those services.

B) Check the files in the below location,

C:\Program Files (x86)\Microsoft SQL Server\MSSQL11.SOTERAEXPRESS\MSSQL\DATA\

- SoteraExpress.mdf
- SoteraLog.mdf

are available.

- **How can I reset Device Configurator application password?**

If you have Administrator access and forgot your password, follow these steps -

- Click the "Windows" icon on the lower left side of your screen.
- Click "All apps."
- Scroll down until you see "Honeywell." Click the downward arrow to see "Unlock Administrator Account."

A. When the "Windows Security" window appears, type in your Administrator password for the PC.

- Click "OK." An activation code is shown.
- Use this activation code to login to Safety Suite Device Configurator.

- **How can I log on to the software if I have forgotten my password?**

You can reset your password by clicking the “Forgot Password” link on the Login Screen. Once you answer the security questions, you will be allowed to reset the password.

➤ **How can I log on to the software if I have locked myself out of the default administrator account?**

You can invoke the “Unlock Administrator Account” utility that is installed with the software to unlock the default administrator account.

- A. For security purposes, you will be prompted to provide the Windows administrator User ID and password before you can unlock the Honeywell Safety Suite Device Configurator administrator account.

Follow the steps to unlock the account –

- A.
- Click the “Windows” icon on the lower left side of your screen.
 - Click “All apps.”
 - Scroll down until you see “Honeywell.” Click the downward arrow to see “Unlock Administrator Account.”
 - When the “Windows Security” window appears, type in your Administrator password for the PC.
 - Click “OK.” An activation code is shown.
 - Use this activation code to login to Safety Suite Device Configurator.

➤ **How to check IIS is running on the machine?**

Follow the steps to check if IIS is running-

- Click on Windows icon. Type “run” in search tab and press Enter.
- Type “inetmgr” and press enter.
- Check if “World Wide Web Publishing Service” is running.
- If not, Check answer to the question “How to enable IIS”.

➤ **How to enable IIS?**

Follow the instructions at - [https://msdn.microsoft.com/en-us/library/ms181052\(v=vs.80\).aspx](https://msdn.microsoft.com/en-us/library/ms181052(v=vs.80).aspx) to enable IIS.

➤ **What is the default username and password for Honeywell Safety Suite Device Configurator?**

The default user name is “administrator”. You are required to create a password for the administrator account when you log into the application for the first time.

A.

➤ **I have entered correct username and password and clicked on login. I am still on login page.**

Check if Device Configurator Database Service is running.

Steps to check and restart the service –

A.

- Click on Windows icon.
- Type run and select run.

A.

- In run windows, type services and press enter.
- Search SafetySuite.DCDataBaseServiceis and check if service status is running. If not, do right click and select restart.

19.4 Device Inventory

➤ **How do I see my instruments in the Device Inventory list?**

For BW instruments connected through IntelliDoX, MicroDock II or IR Dongle, the instrument data should be downloaded for the instruments to show up in the Device Inventory. Make sure the filter option “Not Connected” is selected to view the instruments in the Device Inventory List for which data has been downloaded. For RAE Systems instruments connected through the AutoRAE 2, Travel Charger or Direct USB the software should be able to communicate to the instruments to show up in the Device Inventory list. In addition, instrument data should be downloaded to view the RAE

- A. Systems instruments in the inventory after the instrument is disconnected from the software. The filter option “Not Connected” should be selected to view RAE Systems instruments in the Device Inventory List for which data has been downloaded but are currently not connected to the software.

➤ **What are the different options to connect Docking Stations to the software?**

IntelliDoX can connect to the software over the network. MicroDock II can connect to the software using direct USB connection. AutoRAE 2 can connect to the software either over the network or using direct USB connection.

➤ **I have connected the docking station over the network. However, I am not able to see the docking station in the software?**

First, make sure the software is set up to scan for the RAE Systems and/or BW docking stations by checking the appropriate box for “Allow Dock Discovery” under system Settings. If the docking station is in a network path different than the software, the software may not be able to see the docking station. In order for the software to see the Docking Station, add the Docking Station manually to the software using “Add AutoRAE Controller for manual detection” for AutoRAE 2 and “Add IntelliDoX for manual detection” for IntelliDoX under the system Settings menu option using the IP Address of the Docking

- A. Station.

➤ **I have connected the docking station. However, it is not appearing online in the software.**

The software periodically scans the USB ports and network to check the online status of the docking station/instruments. However, the online status of the docking station might not be reflected right away in the software. If you are unable to see the docking station status online, you can click the Refresh button in the Device Inventory view to see the online status of the docking station.

- A.

- **Can I use the same package to update the firmware for the devices on Honeywell Safety Suite Device Configurator that I use to update the firmware with ProRAE Studio II and Fleet Manager II?**

Honeywell Safety Suite Device Configurator uses digitally signed packages to update the device firmware as a security mechanism to verify the integrity of firmware update packages. As a result, it cannot use the same packages used by ProRAE Studio II and Fleet Manager II. Firmware packages designated for Honeywell Safety Suite Device Configurator should only be used to update device firmware through Honeywell Safety Suite Device Configurator.

- ⚠. **What should be done if devices are connected and not appearing in device inventory list.**

Sometimes the devices might take some time (~ 1-2 mins). If still the problem persists, follow the below steps

- Check if the device is connected correctly.
 - Disconnect and Reconnect the device.
 - Now wait for 2-3 mins.
 - If still the device doesn't appear, use the manual refresh on the device inventory page
- A.
- If still the problem persists, run the services.msc on the Command window and restart all the services related to the Safety Suite.
 - If not, kindly contact the tech support.

- **How can I see only connected or only disconnected devices?**

Use the filter provided on the Left-hand side of the screen and Select the "Connected" or "Disconnected" to filter out the required devices list.

- **What mode should the RAE device be to communicate to Device Configurator?**

Make the RAE in "Communication Mode" to communicate with the Device Configurator. Otherwise the RAE devices won't communicate.

- ⚠. **Do I need driver to connect IR devices in Device Configurator?**

Driver is required to connect IR device. When Device Configurator is installed first time, it asks you to install IR driver while installation. Select yes to install the driver.

- ⚠. **Do I need driver to connect RAE device Configurator?**

Driver is required to connect RAE device. When Device Configurator is installed first time, it asks you to install AutoRAE driver while installation. Select yes to install the driver.

A.

- **Do I need driver to connect IntelliDox device in Device Configurator?**

Driver is not required to connect IntelliDox device.

- ⚠. **How do I check device connected previously?**

From the LHS filter select the "Disconnected" devices to show all the devices which were connected previously.

A.

➤ **How can I archive a device?**

This is a feature whose implementation is still in progress. Expect it in future release of the Application.

19.5 Device Data Download

➤ **Does the software download existing data from the Docking Stations?**

A. The software downloads all the historical data stored in the docking station. The download time can vary depending on the size of the data, network bandwidth and processing speed of the computer.

➤ **I do not see the option to select a start and an end date for data downloaded in Honeywell Safety Suite Device Configurator.**

A. The software utilizes a smart download manager to incrementally download the data to optimize the download time. The software compares the existing downloaded data against the latest logged data and downloads only the incremental data since the last download.

➤ **Does Honeywell Safety Suite Device Configurator support data download from IntelliDox USB connector?**

A. The software supports data download via the USB connector on the IntelliDoX using a USB storage device for BW Clip, BW Clip Real Time, BW MicroClip XL & BW MicroClip X3, BW Clip4, BW Solo, BW Ultra.

➤ **Can I download data of multiple devices at a time in Device Configurator?**

A. Currently, you can only perform data download for one device at a time. You must wait for the current operation to complete before performing another data download.

➤ **How does data Download happen? Do I have initiate it or it happens when devices are discovered in Device Configurator?**

A. Data download does not happen automatically, it must be initiated by user after connecting devices to the application. RAE device, IntelliDox Device and IR should be connected to Device Configurator to initiate data download. When you see the device in Device Inventory, filter the device using serial no and click on "Actions" button. Click on "Download Data" from the options.

➤ **How long should I wait for Data Download to Complete?**

A. If user downloads data first time, it depends on the amount of data available in the device. If user downloads data of the same device again, it downloads the new data only.

➤ **What happens if I disconnect device while data download is in progress?**

A. Device must be connected till data download completes. If device is disconnected while data download is in progress, complete data will not get downloaded and data download failed notification will appear on the screen.

19.6 Device Configuration

- **Why am I not able to save the Dock/Device Configuration?**
To perform the Dock/Device Configuration, the Dock /Device needs to be connected to the computer and appear online to the software.
- **Can I download data and configure a device at the same time?**
Currently, you can only perform one device action at a time. You must wait for the current operation to complete before performing another action. Consequently, if you are performing a data download, you must wait for the data download to complete before performing a device configuration.
A.
- **For BW devices, unlike Fleet Manager, I do not see the Updatable option against each of the sensor parameters. Why?**
A. Honeywell Safety Suite Device Configurator has a streamlined user interface to make it easier to manage configuration parameters. As a result, a common Updatable option is provided for all of the configuration parameters, including the sensor settings, under the Settings tab.
- **For RAE Systems devices, can I update the Lot Number of the gas cylinder in the software?**
A. You can navigate to the AutoRAE 2 details and edit the gas inlet configuration details for the attached gas cylinder in order to update the Lot Number of the gas cylinder.
- **For RAE Systems devices, can I update the Sensor Serial No. after installing a new sensor?**
Yes, you can update the Sensor Serial No. of RAE devices after installing a new sensor for the instruments that support this option under the Sensors tab for the corresponding instruments if they are currently online and connected to the software.
A.
- **Does Honeywell Safety Suite Device Configurator support instrument configuration use IntelliDox USB connector?**
The software supports instrument configuration via the USB connector on the IntelliDox using a USB storage device for BW Clip, BW Clip Real Time, BW MicroClip XL & BW MicroClip X3, BW Clip4, BW Solo, BW Ultra.
A.
- **I am unable to save configuration in MicroDock. What should I do?**
PC where MicroDock is connected must have write access to USB connected devices. Verify if you have the access. MicroDock creates a temporary drive on the PC when connected and read and write operation happens on the same drive.
A.

19.7 Device History

- **What information is presented in Device History?**
A.

Device History provides a comprehensive view of all the data related to the lifecycle of the selected instrument. This includes test data for calibration and bump tests. This also includes the instrument event data, along with the corresponding data logs.

➤ **Are all device-related data logs, event logs and test data logs shown in the Device History?**

All information related to device data logs, event logs and test logs is shown in the

- A. Device History, with the exception of IntelliDoX & MicroDock II data logs and BW instrument test logs for bump and calibration operations performed outside of the IntelliDoX & MicroDock II.

➤ **Why can't I see the Device History?**

Make sure that you have downloaded the data from the docking station corresponding to

- A. the selected instrument before viewing the Device History. Once the data has been downloaded, you can view the history for the selected device.

➤ **Can I export the data log corresponding to the events captured by the instrument?**

Yes, you can export the instrument data log in csv (comma-separated value) format, which can be opened in Microsoft Excel for further analysis.

A.

➤ **Can I delete the data log for an instrument once it has been imported into the software?**

We do not allow data logs to be deleted once they have been downloaded to the software.

A.

➤ **What is the maximum date range in I can select in calendar to see Device History?**

The maximum date range that can be selected in calendar is 1 year, at any given point of time. However, the user can select any date range of maximum one year up to current date. For ex: User can select the date range of 1-1-2013 to 31-12-2013 in Calendar.

A.

19.8 User Management

➤ **What are the different roles I can assign to a user?**

- A. You can assign one or more of the following roles to a user:

Administrator – A user with the administrator role has access to all the features and functionality within the system.

Advanced User – A user with the advanced role can perform all the device operations. However, the user does not have access to user management.

- A. Standard User – A user with the standard role can perform all device operations except device configuration and firmware updates.

Worker – A user with the worker role has no access to the software. However, the user can be assigned/unassigned instruments.

➤ **I want to assign an instrument to an individual. However, I do not want to provide the individual with access the software.**

You can assign a user the “Worker” role if you want to just assign instruments to the user.

➤ **What is the purpose of deactivating a user account?**

If you want to temporarily suspend user access to the system, you can do that by deactivating the user account.

⚠. **Can I change the username of the admin user in Device Configurator?**

No, username of the admin user cannot be updated.

➤ **How do I update the admin user profile?**

A. Follow the steps to update the profile -

○ Login to the application. Click on the User icon available on the right side of the top header.

A. ○ Select “Edit Profile”.

○ Update the user profile fields which are updatable.

○ To save the updated profile, click Save button.

A.

➤ **How do I update user profile of the users other than the admin user?**

Follow the steps to update the profile -

○ Login to the application. Click on the User icon available on the left-hand side bar on the Inventory page.

○ Filter the user with username or name of the user.

○ Click on “Actions” button of the username. Select “User details”.

○ Update the user profile fields which are updatable.

A. ○ To save the updated profile, click Save button.

19.9 Data Migration

➤ **Can BW device data be migrated when both FM and Device Configurator Running?**

No, we cannot migrate the data when FM and Device Configurator are running. We can migrate data to Device configurator after closing FM.

➤ **Can I migrate IntelliDox and MicroDock data log in Device Configurator?**

No, we cannot Migrate IntelliDox and MicroDock data log in Device configurator. Data log of the devices docked in IntelliDox and MicroDock can only be migrated.

⚠. **Does a device which has no data get migrated?**

We cannot migrate a device which does not have any data.

➤ **Why do I see the difference in date and time of the data logs in FM and Device Configurator?**

A. FM shows the data in UTC format, in Device Configurator the data is shown in the local time zone of the computer where it is installed.

A.

- **How can I migrate custom fields from FM to Device Configurator?**
Yes, we can migrate custom fields from FM to Device Configurator. In case of custom fields in FM then move this “Userdef.properties” file from data folder to database folder in FM migration.
- **How can I migrate data log, event log and results from PRS to Device Configurator?**
Launch the Device configurator and login as Administrator.
 - A.
 - Navigate to “Data migration” dropdown option in the User tab\option in top right menu of the application.
 - Select the software "ProRae Studio".
 - In the “Data Source Folder”: Click “ADD FOLDER”
 - Now select the path of the PRS files folder. (Note: keep the files in the path other than Desktop)
 - Then “MIGRATE” Button will be enabled.
 - Click “MIGRATE”
 - The Migration process starts and the user will be notified after the migration is completed.
- **How can I migrate data log, event log and results from FM to Device Configurator?**
Launch the Device configurator and login as Administrator.
 - A.
 - Navigate to “Data migration” dropdown option in the User tab\option in top right menu of the application.
 - Select the software "Fleet Manager".
 - In the “Data Source Folder”: Click “ADD FOLDER”
 - Now select the path of the Root folder where all the FM Device files are placed. (Note: keep the files in the path other than Desktop)
 - Then “MIGRATE” Button will be enabled.
 - Click “MIGRATE”
 - The Migration process starts and the user will be notified after the migration is completed.
- **How can I migrate data log, event log and results from IQ Manager to Device Configurator?**
Launch the Device configurator and login as Administrator.
 - A.
 - Navigate to “Data migration” dropdown option in the User tab\option in top right menu of the application.
 - Select the software "IQ Manager".
 - In the “Data Source Folder”: Click “ADD FOLDER”
 - Now select the path of the IQ Manager DB Server details.
 - Then “MIGRATE” Button will be enabled.

- Click “MIGRATE”
 - The Migration process starts and the user will be notified after the migration is completed.
- **Can I do selective data migration of users only, data log only, custom field only?**
There is no option to select a type of data for migration. Complete data is migrated when migration is done.
- **FM is installed but I do not see FM data folder, what should I do to access the data folder?**
Data folder is hidden. To see the folder, follow the steps -
- A.
 - Navigate to computer drive “C:\ “and set “show hidden files and folders” in view .
 - Then Programdata folder will be visible, the files can be seen in below path.
 - “C:\ProgramData\BW Technologies\Fleet Manager II\data\database” folder
- **Where should I keep data migration files for successful migration?**
A. The Data files should be placed in a folder other than the Desktop or the path where the Folder has the permissions to get retrieved by Device Configurator.
- **How long should I wait for Data Migration to complete?**
Depends on the Data present in the files. (Max 4 hours.)
- **What files are supported for Data Migration?**
A. Files supported for Data Migration are
 - Properties, .Script, .Data, .fmdl extension files are supported for FM.
 - .prs for Proraestudio.
- A.
 - IQ manager connects to DB directly.
- **What different type of data can be migrated from FM to Device Configurator?**
A. We can migrate Data log, Test log, Event log, Users, Custom fields.
- **What different type of data can be migrated from PRS to Device Configurator?**
We can migrate Data log, Test log, Event log fields.
- **What different type of data can be migrated from IQ Manager to Device Configurator?**
A. We can migrate Data log, Test log, Event log.
- **I am not able to select the folder for data migration. What should I do?**
A. Check the folder has permissions to be selectable, once permissions are given the folder will be selectable.
- **Can I migrate data from Device Configurator to Device Manager, FM, PRS, IQ Manager?**
A. **Manager?**
No, we cannot migrate.

A.

➤ **Notes for Data Migration –**

- In case of custom fields in FM then move this “Userdef.propertyed” file from data folder to database folder in FM migration.
- Close FM before initiating the DB migration.
- Recommended that if there are any data log file then archive then migrate.
- Do not perform any other operations like data download while data migration is in progress.
- Large file migration – need to check at service side about segregation.
- Default Intellidox Date/Time UTC, same will be shown when downloaded in FM. Hence data shown in FM assumed as UTC and get converted to locale date/time in DC/DM.
- FM: Intellidox and Microdock data also appears against the respective devices.
- Devices having data and Users assigned with devices alone will get migrated.
- IQ Manager data migration – First time migration does the full migration, subsequent migration do only delta data based on set interval.

19.10 Firmware

➤ **What all firmware versions are supported in RAE?**

Device Firmware Version supported in Safety Suite.

A.

Product Name	Model No	Version Name
AreaRAE Pro	PGM-6560	v1.08
AutoRAE 2 Controller	*	v1.34
Handheld PID Cradle	DKS-6004	v1.34
MicroRAE	*	v1.10
MicroRAE Cradle	*	v1.32
MiniRAE 3000	PGM-7320	v2.16
MiniRAE Lite	PGM-7300	v2.16
MultiRAE	*	v1.40.C
MultiRAE Cradle	*	v1.32
MultiRAE Lite	*	v1.40.C
MultiRAE Lite Sensor	*	v1.40.C
MultiRAE Pro	*	v1.40.C
MultiRAE Pro Sensor	*	v1.40.C
MultiRAE Sensor	*	v1.40
MultiRAE WiFi	*	v1.36
MultiRAE WTK	*	v1.32

ppbRAE 3000	*	v2.16
ppbRAE 3000	PGM-7340	v2.16
QRAE 3	*	v2.12
QRAE 3 Cradle	*	v1.32
ToxiRAE Pro	*	v1.80
ToxiRAE Pro CO2	*	v1.80
ToxiRAE Pro Cradle	DKS-6002	v1.32
ToxiRAE Pro LEL	*	v1.80
ToxiRAE Pro PID	*	v1.80
UltraRAE 3000	PGM-7360	v2.16

➤ **What all firmware versions are supported in BW?**

Device Firmw are Version supported in Safety Suite.

A.

Product Name	Model No	Version Name
BW Clip	*	v2.0
BW Clip4	*	v1.340
BW Solo	*	v01.001
BW Ultra	*	v00.950
GasAlertMax XT	*	v12.000
GasAlertMicroClip	*	v50.0
GasAlertQuattro	*	v04.000
Handheld PID Cradle	DKS-6004	v1.34
IntelliDoX	GasAlertMicroClip	v8.0
IntelliDoX	BWSolo	v9.016
IntelliDoX	BWClip4	v09.012
IntelliDoX	BWClip	v9.012
IntelliDoX	BWUltra	v09.012
IntellidoxForBWClip	*	v9.012
IntellidoxForBWClip4	*	v8.000
IntelliDoXForBWSolo	*	v09.016
IntelliDoXForBWUltra	*	v9.012
IntellidoxForMicroClip	*	v8.000

- **How do I upgrade device firmware manually?**
Follow the steps to upgrade firmw are manually -
 - Go to the device details
 - Disconnect from the internet
 - Now Click the “Update” option below the Firmw are Version
 - On the Popup Window , Select the Firmw are version w hich you would like to have
 - Select the correct Firmw are file (RFP files)
- A.
 - Wait till the Firmw are gets upgraded

Note: Firmw are can be upgraded only if the device is not on the latest Firmw are
- **Where can I find the firmware files?**
You can find the related product firmw are in Product Registration Module (PRM).
- **Firmware update fails on clicking UPDATE on device details page.**
This happens due to Product Registration Module (PRM) server not working. Try the update later. Contact Tech Support for further assistance.
- **When I click on UPDATE on device details page, it asks me to upload a firmware file. It should update the firmware automatically. What is wrong?**
This happens due to Product Registration Module (PRM) server not w orking. Try the update later or update the firmw are w ith the supported firmw are file. Contact Tech Support for further assistance.
- **Device firmware version is latest and I see “UPDATE” button enabled on device details page. Do I need to upgrade the firmware?**
This happens due to Product Registration Module (PRM) server not w orking. Contact Tech Support for further assistance.

19.11 Passcode

- **What is the purpose of Network Passcode, Menu Passcode and IntelliDox Web passcode?**
A.
 - **Network Passcode:** To Secure the IntelliDoX data from unauthorized access in the Safety Suite.
 - **Menu Passcode:** To Secure the IntelliDoX Menu from unauthorized access in the IntelliDoX.
 - **IntelliDoX Web Passcode:** To View and Modify the Netw ork Parameters and IntelliDox Information of IntelliDoX.
- **When passcode is required for IntelliDox?**
Passcode is required to access the IntelliDoX for version 9.0 or above.
- **How does Passcode work when IntelliDox firmware is upgraded?**
Passcode w ould be retained even if the IntelliDoX firmw are is upgraded.

➤ **Why am I not able to perform “Device Details” and “Data Download” options in the instrument list view for some of the IntelliDoX?**

A. To perform “Device Details” and “Data Download” in the instrument list view, you should provide the network passcode to IntelliDoX for version 9.0 or above.

➤ **Where can I view the network Passcode in Device Configurator?**

You cannot view the Passcode in Device Configurator.

➤ **Can I configure network Passcode through Device Configurator?**

Yes, you can configure the Network Passcode.

- After the IntelliDoX is visible as Connected in Device Discovery Page
- Go to the Actions drop-down and Select the “Set Passcode”.

A. ○ Provide the same passcode as the one in IntelliDoX and click Continue.

○ The Message will appear, whether the provided passcode is correct, or not.

○ After this the operation remains the same as before.

A.

19.12 Language Support

➤ **Does Device Configurator application text appear in languages other than English?**

No, Currently Device Configurator application will display text only in English irrespective of the base OS Language or Locale/ Chrome browser settings being set.

➤ **Can I give data inputs in language other than English?**

No, currently data inputs can be given only as per US English language format.

Ex: Decimal notation will be “.” So sensor values will be in the form “12.7”.

➤ **If I my PC OS is not English, Can I use Device Configurator?**

Yes, even if PC OS is not in English, Device Configurator application can be launched and used. The language inputs and text will still be in English though.

➤ **What languages are currently supported by Honeywell Safety Suite Device Configurator?**

Currently only English language is being supported by Safety Suite Device Configurator.

19.13 Device Registration

➤ **How do I register a device in Device Configurator?**

Follow the steps to register a device:

A. ○ Login to the Device Configurator.

○ Inventory page header has a device icon. Click on the icon.

○ The devices connected will appear in the registration window.

○ Click on the register button to register the devices.

A.

Note: To register devices automatically, select checkbox “Register new devices automatically”.

19.14 Event Report

➤ **How do I generate event report?**

Follow the below steps:

- Go to the Reporting Tab on the LHS on the Device Inventory page
- Select the “Event Log” in the Report type
- Select the date range for which the report needs to be generated
- Then select the Device Serial number from the drop-down and click Generate.
- A pdf file of the report will be generated in the Notification.

A.

➤ **What is the maximum date range I can select to generate report?**

The maximum date range that can be selected in calendar is 1 year, at any given point of time. However, the user can select any date range of maximum one year up to current date.

For ex: User can select the date range of 1-1-2013 to 31-12-2013 in Calendar

A.

Revision: 2.1.1



THE POWER OF **CONNECTED**

For more information

www.honeywellanalytics.com

www.raesystems.com

<p>Europe, Middle East, Africa Life Safety Distribution GmbH Tel: 00800 333 222 44 (Free phone number) Tel: +41 44 943 4380 (Alternative number) Fax: 00800 333 222 55 Middle East Tel: +971 4 450 5800 (Fixed Gas Detection) Middle East Tel: +971 4 450 5852 (Portable Gas Detection) gasdetection@honeywell.com</p>	<p>Americas Honey well Analytics Distribution Inc. Tel: +1 888 749 8878 Fax: +1 817 274 8321 detectgas@honeywell.com</p> <p>Honey well RAE Systems Phone: 408 952 8200 Toll Free: 1 888 723 4800 Fax: 408 952 8480</p>	<p>Asia Pacific Honey well Analytics Asia Pacific Tel: +82 (0) 2 6909 0300 Fax: +82 (0) 2 2025 0328 India Tel: +91 124 4752700 analytics.ap@honeywell.com</p> <p>Technical Support support.safetysuite@honeywell.com 1-833-556-3515</p>
-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------	--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------	------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------